

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007795.D
 Acq On : 23 Sep 2018 18:02
 Operator : SY/MD
 Sample : J5010-05
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0T11

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	68	72	79	rVB	6166	5732	9.28%	1.494%
2	1.589	151	155	160	rVB	5531	5133	8.31%	1.338%
3	2.139	318	326	341	rVB2	10871	15874	25.71%	4.137%
4	2.309	372	379	392	rVB3	1579	2702	4.38%	0.704%
5	2.978	584	587	590	rBV	213	112	0.18%	0.029%
6	3.061	610	613	614	rBV	186	91	0.15%	0.024%
7	3.094	621	623	627	rVB3	184	113	0.18%	0.029%
8	3.164	643	645	647	rBV	176	92	0.15%	0.024%
9	3.254	670	673	674	rBV	146	86	0.14%	0.022%
10	3.299	685	687	690	rVB	189	72	0.12%	0.019%
11	3.409	718	721	723	rBV	152	69	0.11%	0.018%
12	3.553	760	766	769	rBV	94	105	0.17%	0.027%
13	3.849	852	858	861	rBV	183	247	0.40%	0.064%
14	3.952	878	890	913	rBV3	2504	8521	13.80%	2.220%
15	4.068	924	926	928	rVB	152	46	0.07%	0.012%
16	4.090	930	933	936	rVV	164	75	0.12%	0.020%
17	4.126	941	944	946	rBV	95	58	0.09%	0.015%
18	4.290	992	995	1001	rVB	97	61	0.10%	0.016%
19	4.412	1018	1033	1048	rBV2	7973	18432	29.85%	4.803%
20	4.540	1072	1073	1075	rVB2	133	46	0.07%	0.012%
21	5.106	1232	1249	1264	rBV4	17917	43131	69.85%	11.239%
22	5.264	1295	1298	1301	rBV	68	57	0.09%	0.015%
23	5.351	1322	1325	1332	rBV	86	106	0.17%	0.028%
24	5.521	1375	1378	1380	rBV	153	136	0.22%	0.035%
25	5.627	1407	1411	1414	rBV2	142	130	0.21%	0.034%
26	5.672	1414	1425	1437	rBV2	17695	33246	53.84%	8.663%
27	5.798	1462	1464	1465	rBV2	128	50	0.08%	0.013%
28	5.904	1494	1497	1502	rVB	205	121	0.20%	0.032%
29	5.968	1505	1517	1534	rBV2	31843	61745	100.00%	16.090%
30	6.126	1555	1566	1581	rVB4	10176	18746	30.36%	4.885%
31	6.351	1635	1636	1641	rVB	128	45	0.07%	0.012%
32	6.408	1652	1654	1656	rBV	135	99	0.16%	0.026%
33	6.621	1715	1720	1723	rBV	186	236	0.38%	0.061%
34	6.823	1778	1783	1785	rBV	102	90	0.15%	0.023%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007795.D
 Acq On : 23 Sep 2018 18:02
 Operator : SY/MD
 Sample : J5010-05
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0T11

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

35	6.965	1824	1827	1831	rBV	112	96	0.16%	0.025%
36	7.042	1840	1851	1860	rBV2	3654	6510	10.54%	1.696%
37	7.138	1877	1881	1888	rBV	99	138	0.22%	0.036%
38	7.286	1923	1927	1931	rVB2	153	120	0.19%	0.031%
39	7.367	1941	1952	1964	rBV2	18926	33228	53.81%	8.659%
40	7.437	1972	1974	1977	rVB	241	119	0.19%	0.031%
41	7.466	1977	1983	1986	rBV2	176	153	0.25%	0.040%
42	7.634	2033	2035	2039	rBV	73	52	0.08%	0.014%
43	7.672	2039	2047	2055	rBV5	2098	3432	5.56%	0.894%
44	7.888	2111	2114	2118	rBV	70	68	0.11%	0.018%
45	7.984	2143	2144	2147	rVB	131	51	0.08%	0.013%
46	8.026	2147	2157	2169	rVB2	14371	24005	38.88%	6.255%
47	8.106	2177	2182	2186	rBV	99	111	0.18%	0.029%
48	8.154	2186	2197	2212	rBV5	3254	9321	15.10%	2.429%
49	8.338	2253	2254	2257	rVB5	129	48	0.08%	0.013%
50	8.379	2264	2267	2269	rBV	69	44	0.07%	0.011%
51	8.418	2278	2279	2281	rVB	126	44	0.07%	0.011%
52	8.434	2281	2284	2288	rBV	106	66	0.11%	0.017%
53	8.617	2338	2341	2346	rBV	69	60	0.10%	0.016%
54	8.904	2420	2430	2446	rBV2	19502	32645	52.87%	8.507%
55	9.045	2471	2474	2481	rBV	99	122	0.20%	0.032%
56	9.457	2599	2602	2604	rBV	79	59	0.10%	0.015%
57	9.878	2730	2733	2738	rVB	96	79	0.13%	0.021%
58	10.010	2772	2774	2779	rVB	178	103	0.17%	0.027%
59	10.267	2844	2854	2867	rBV3	11684	18332	29.69%	4.777%
60	10.485	2919	2922	2926	rBV	100	89	0.14%	0.023%
61	10.595	2954	2956	2959	rVB	170	62	0.10%	0.016%
62	10.727	2995	2997	3000	rVB	158	51	0.08%	0.013%
63	10.794	3015	3018	3020	rBV	91	63	0.10%	0.016%
64	10.878	3041	3044	3046	rBV	141	64	0.10%	0.017%
65	11.064	3099	3102	3105	rVB	206	98	0.16%	0.026%
66	11.174	3134	3136	3140	rVB	137	74	0.12%	0.019%
67	11.305	3167	3177	3189	rBV2	10493	17149	27.77%	4.469%
68	11.357	3192	3193	3196	rVB2	154	56	0.09%	0.015%
69	11.376	3196	3199	3203	rBV	139	75	0.12%	0.020%
70	11.402	3204	3207	3210	rBV	92	69	0.11%	0.018%
71	11.566	3255	3258	3261	rVV2	141	124	0.20%	0.032%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
 Data File : VV007795.D
 Acq On : 23 Sep 2018 18:02
 Operator : SY/MD
 Sample : J5010-05
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0T11

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

72	11.585	3261	3264	3267	rVB2	179	159	0.26%	0.041%
73	11.617	3268	3274	3278	rBB2	204	209	0.34%	0.054%
74	11.682	3284	3294	3305	rBV2	11778	18310	29.65%	4.771%
75	11.871	3350	3353	3355	rBV2	125	80	0.13%	0.021%
76	11.926	3366	3370	3375	rBV2	212	173	0.28%	0.045%
77	11.997	3391	3392	3394	rVB2	144	50	0.08%	0.013%
78	12.045	3404	3407	3411	rBV	210	171	0.28%	0.045%
79	12.064	3411	3413	3414	rBV	167	75	0.12%	0.020%
80	12.138	3435	3436	3438	rBV	100	56	0.09%	0.015%
81	12.170	3444	3446	3448	rBV	123	71	0.11%	0.019%
82	12.215	3456	3460	3463	rVB	166	105	0.17%	0.027%
83	12.260	3472	3474	3476	rVB2	157	80	0.13%	0.021%
84	12.299	3484	3486	3488	rBV2	143	86	0.14%	0.022%
85	12.328	3493	3495	3496	rBV2	115	46	0.07%	0.012%
86	12.341	3497	3499	3502	rVB2	134	72	0.12%	0.019%
87	12.363	3502	3506	3509	rBV2	165	119	0.19%	0.031%
88	12.453	3531	3534	3535	rBV	134	90	0.15%	0.023%
89	12.569	3567	3570	3572	rBV2	123	92	0.15%	0.024%
90	12.611	3581	3583	3585	rVB	161	64	0.10%	0.017%
91	12.627	3585	3588	3589	rBV	192	132	0.21%	0.034%
92	12.739	3620	3623	3624	rBV	176	113	0.18%	0.029%
93	12.810	3643	3645	3647	rBV2	125	85	0.14%	0.022%
94	12.862	3659	3661	3663	rBV2	111	56	0.09%	0.015%
95	13.074	3726	3727	3731	rBV2	109	78	0.13%	0.020%
96	13.309	3798	3800	3801	rBV	172	58	0.09%	0.015%
97	13.730	3929	3931	3934	rVB	245	79	0.13%	0.021%
98	14.553	4185	4187	4190	rBV2	269	149	0.24%	0.039%
99	14.862	4281	4283	4286	rBV3	375	170	0.28%	0.044%
100	14.903	4294	4296	4298	rBV	305	136	0.22%	0.035%


Sum of corrected areas: 383749

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092318\
Data File : VV007795.D
Acq On : 23 Sep 2018 18:02
Operator : SY/MD
Sample : J5010-05
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
COT11

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

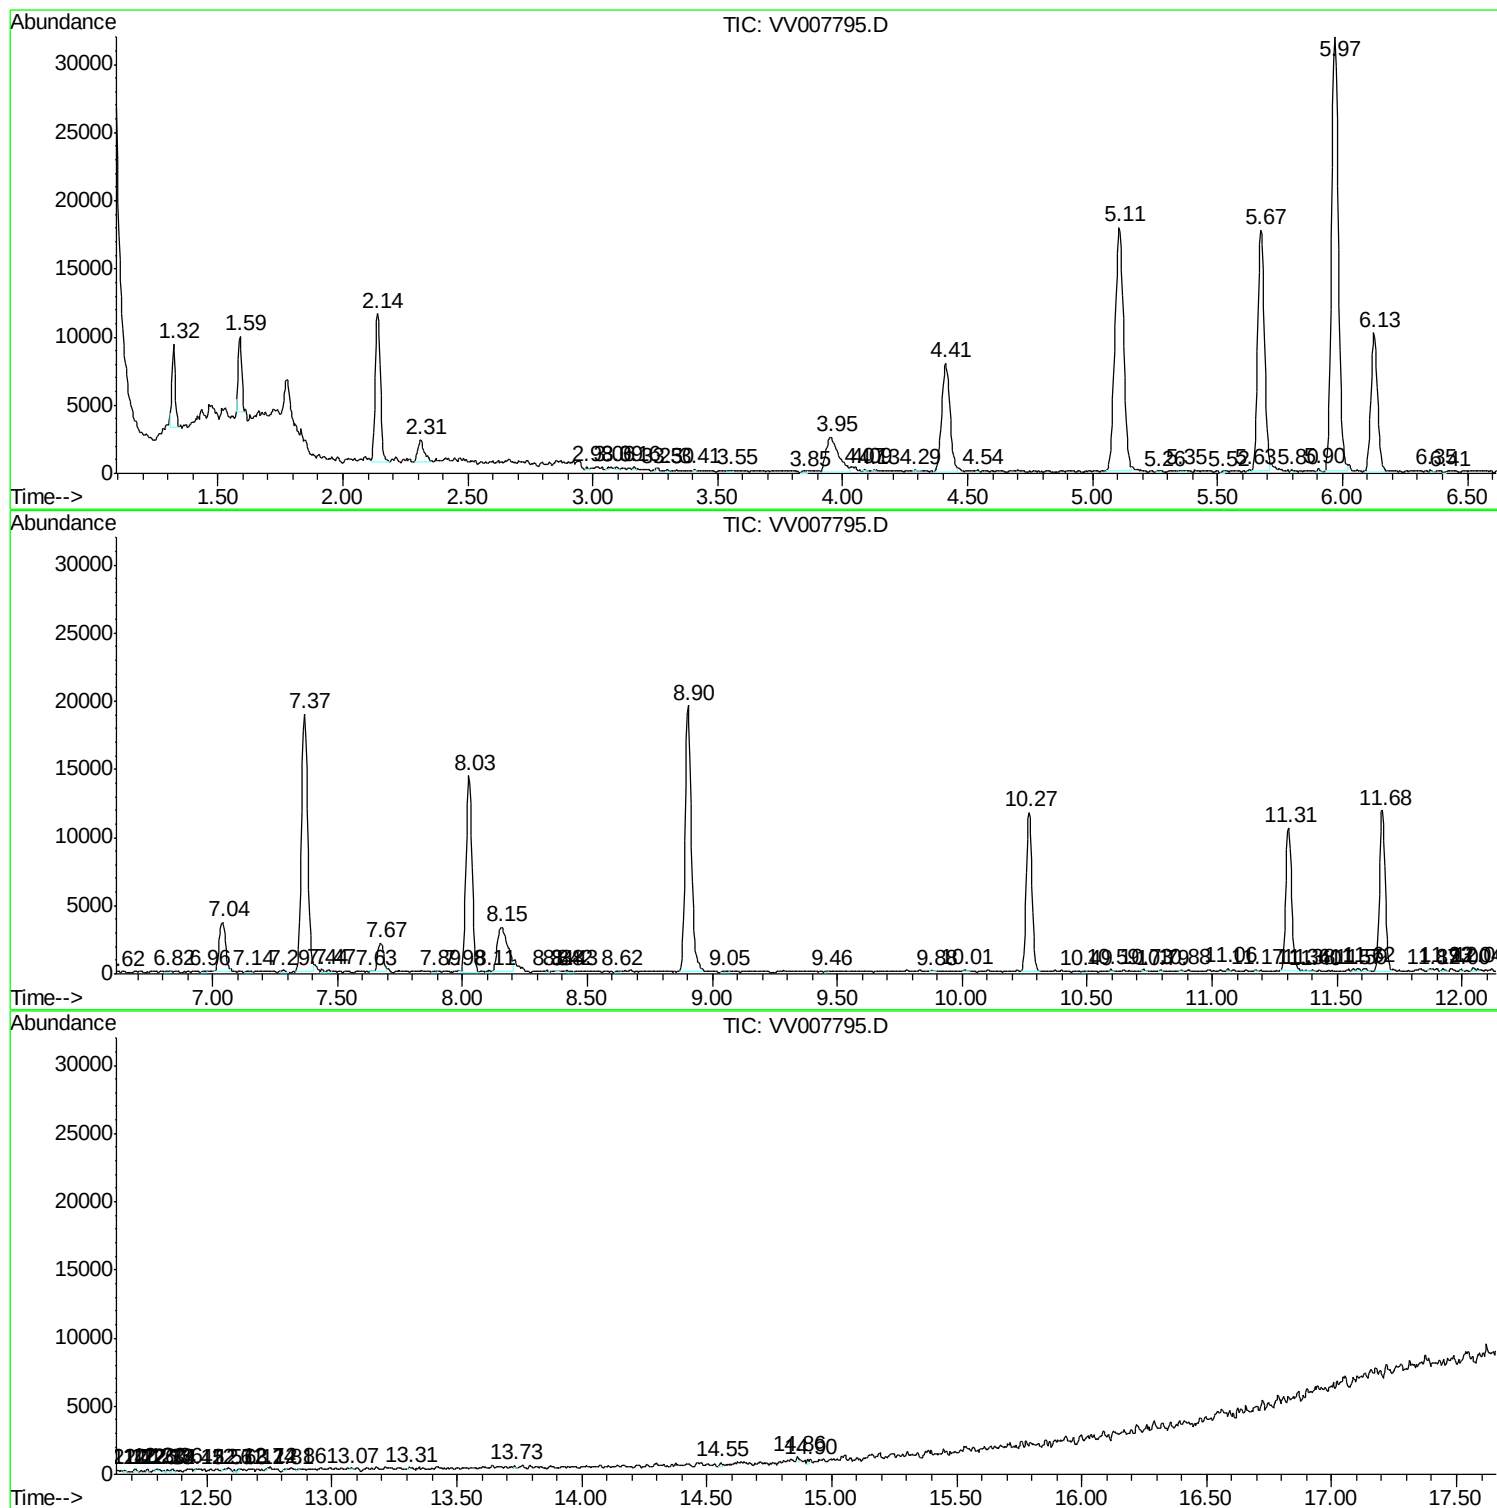

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV092318\
Data File : VV007795.D
Acq On : 23 Sep 2018 18:02
Operator : SY/MD
Sample : J5010-05
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0T11

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV092318\
Data File : VV007795.D
Acq On : 23 Sep 2018 18:02
Operator : SY/MD
Sample : J5010-05
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 73 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0T11

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc