


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092318\
Data File : VV007729.D
Acq On : 22 Sep 2018 11:39
Operator : SY/MD
Sample : BFB71
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB71

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Title : VOC Analysis
Last Update : Tue Sep 25 04:04:32 2018

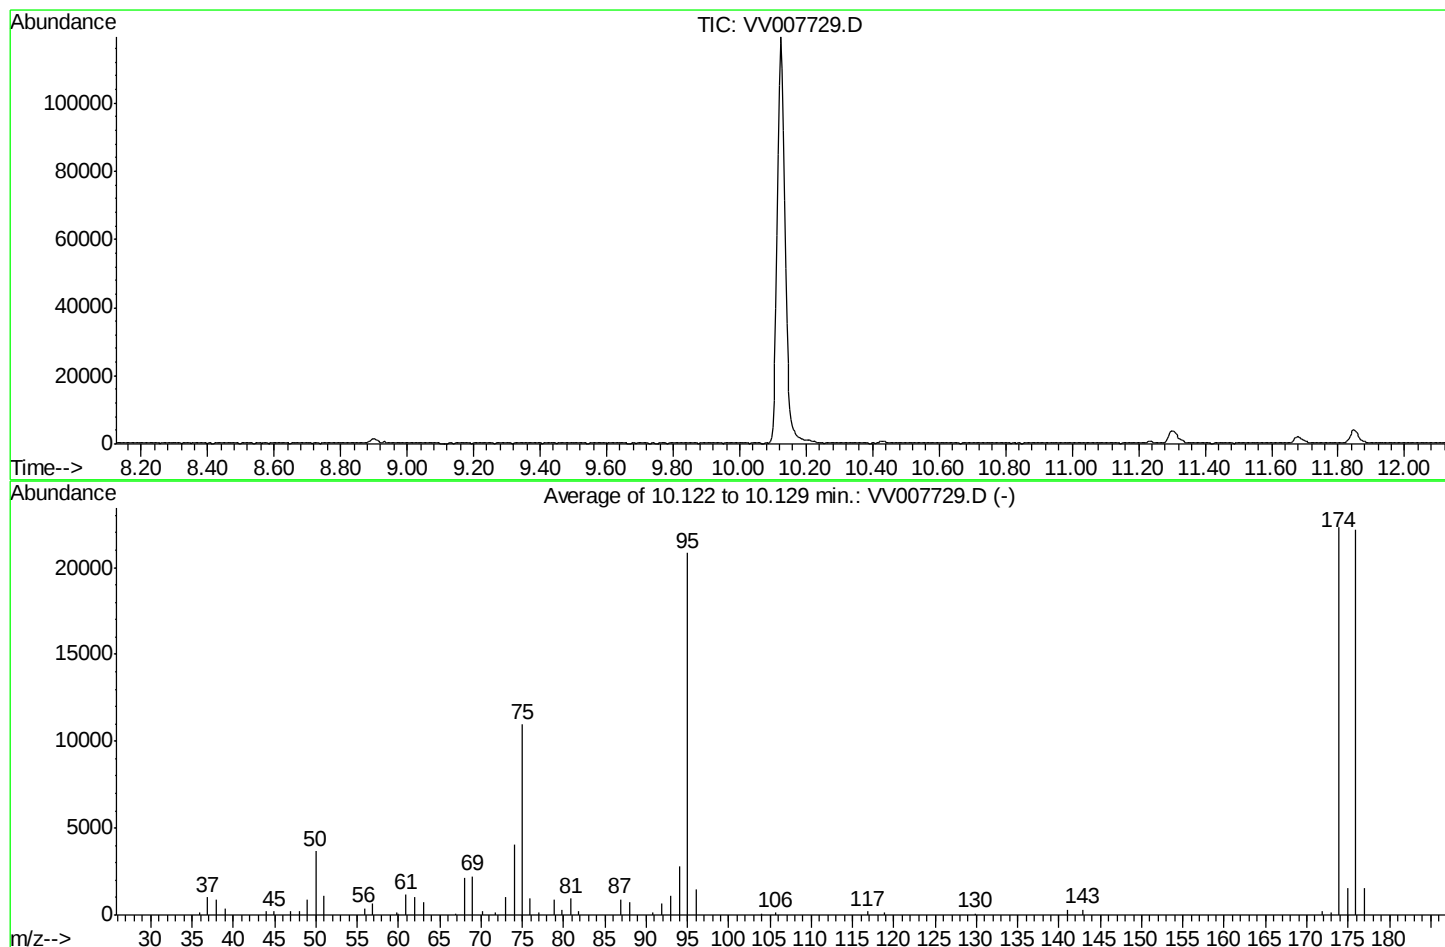

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	3682	PASS
75	95	30	80	52.6	10971	PASS
95	95	100	100	100.0	20842	PASS
96	95	5	9	7.2	1498	PASS
173	174	0.00	2	0.6	144	PASS
174	95	50	120	107.1	22317	PASS
175	174	5	9	7.1	1579	PASS
176	174	95	101	99.5	22197	PASS
177	176	5	9	6.8	1520	PASS

m/z	Abundance
43.90	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	181.0
36.90	990.0
37.90	952.0
38.90	413.0
44.00	395.0
44.90	204.0
47.00	239.0
47.90	188.0
49.00	870.0
50.00	3790.0
51.00	1238.0
55.90	460.0
56.90	686.0
59.80	211.0
61.00	1240.0
62.00	1079.0
63.00	801.0
66.90	122.0
68.00	2213.0
69.00	2308.0
70.10	218.0
71.80	178.0
73.00	1101.0
74.00	4101.0
75.00	11244.0
76.00	999.0
77.00	157.0
78.90	915.0
79.80	338.0
80.90	1002.0
81.80	260.0
86.90	925.0
87.90	703.0
90.90	116.0
91.90	694.0
92.90	1090.0
94.00	2837.0
95.00	21256.0
96.00	1503.0
103.90	134.0
105.70	116.0
116.90	188.0
118.80	156.0
129.90	144.0
140.90	279.0
142.90	306.0
171.90	211.0
173.90	22352.0
174.90	1566.0
175.90	22208.0
176.90	1574.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	164.0
36.90	1066.0
38.00	880.0
38.90	378.0
44.00	379.0
44.90	222.0
47.00	240.0
47.90	211.0
49.00	875.0
50.00	3722.0
51.00	1121.0
55.90	411.0
56.90	659.0
59.80	189.0
60.90	1232.0
61.90	1075.0
63.00	762.0
67.00	105.0
68.00	2166.0
69.00	2287.0
70.10	224.0
71.80	181.0
73.00	1049.0
74.00	4233.0
75.00	11361.0
75.90	967.0
76.90	163.0
78.90	933.0
79.80	335.0
80.90	980.0
81.80	231.0
86.90	961.0
87.90	738.0
90.80	136.0
91.90	703.0
92.90	1125.0
94.00	2878.0
95.00	21576.0
96.00	1558.0
103.90	113.0
105.80	123.0
116.90	204.0
118.80	147.0
129.90	124.0
141.00	304.0
142.90	328.0
171.80	232.0
172.90	223.0
173.90	23080.0
174.90	1609.0
175.90	22888.0
176.90	1579.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
35.90	146.0
36.90	1002.0
38.00	770.0
39.00	327.0
44.00	379.0
45.00	209.0
47.00	204.0
48.00	182.0
49.00	814.0
50.00	3535.0
51.00	969.0
55.90	327.0
56.90	604.0
59.80	151.0
60.00	150.0
60.90	1057.0
61.90	1013.0
63.00	706.0
68.00	1952.0
68.90	2074.0
70.10	190.0
71.80	146.0
73.00	921.0
74.00	3848.0
75.00	10309.0
75.90	869.0
76.90	168.0
78.90	876.0
79.80	288.0
80.90	891.0
81.90	202.0
86.90	876.0
88.00	728.0
90.80	130.0
91.90	644.0
93.00	1036.0
94.00	2626.0
95.00	19696.0
96.00	1433.0
105.80	110.0
116.90	194.0
118.80	133.0
140.90	290.0
142.90	328.0
171.80	240.0
173.00	209.0
173.90	21520.0
174.90	1563.0
175.90	21496.0
176.90	1409.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71