

Data File : VV012942.D
Acq On : 23 Sep 2019 17:49
Operator : SY/MD
Sample : K4958-08
Misc : 3.36G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESNY4

Quant Time: Sep 24 07:42:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 24 07:38:53 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	612960	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	465586	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	104362	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	246261	25.89	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.56%
7) Chloroethane-d5	1.58	69	218964	28.48	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	113.92%
10) 1,1-Dichloroethene-d2	2.13	63	322265	20.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.52%
20) 2-Butanone-d5	3.95	46	106128	32.32	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.64%
24) Chloroform-d	4.40	84	440532	26.16	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	104.64%
26) 1,2-Dichloroethane-d4	5.08	65	251613	25.71	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.84%
29) Benzene-d6	5.10	84	913520	35.14	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	140.56%#
33) 1,2-Dichloropropane-d6	6.12	67	287749	35.32	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	141.28%#
37) Toluene-d8	7.36	98	706047	29.92	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	119.68%
38) trans-1,3-Dichloropropene-	7.66	79	74394	21.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.24%
39) 2-Hexanone-d5	8.14	63	56389	34.39	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.78%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	165634	21.40	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.60%
61) 1,2-Dichlorobenzene-d4	11.67	152	104652	25.81	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.24%


Target Compounds					Qvalue
13) Acetone	2.21	43	68851	19.726 ug/L	100
16) Methylene chloride	2.54	84	53759	5.868 ug/L	98
49) 2-Hexanone	8.17	43	37154	8.902 ug/L #	36
59) 1,2,3-Trichloropropane	11.29	75	12708	2.175 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV012942.D
Acq On : 23 Sep 2019 17:49
Operator : SY/MD
Sample : K4958-08
Misc : 3.36G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESNY4

Quant Time: Sep 24 07:42:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 24 07:38:53 2019
Response via : Initial Calibration

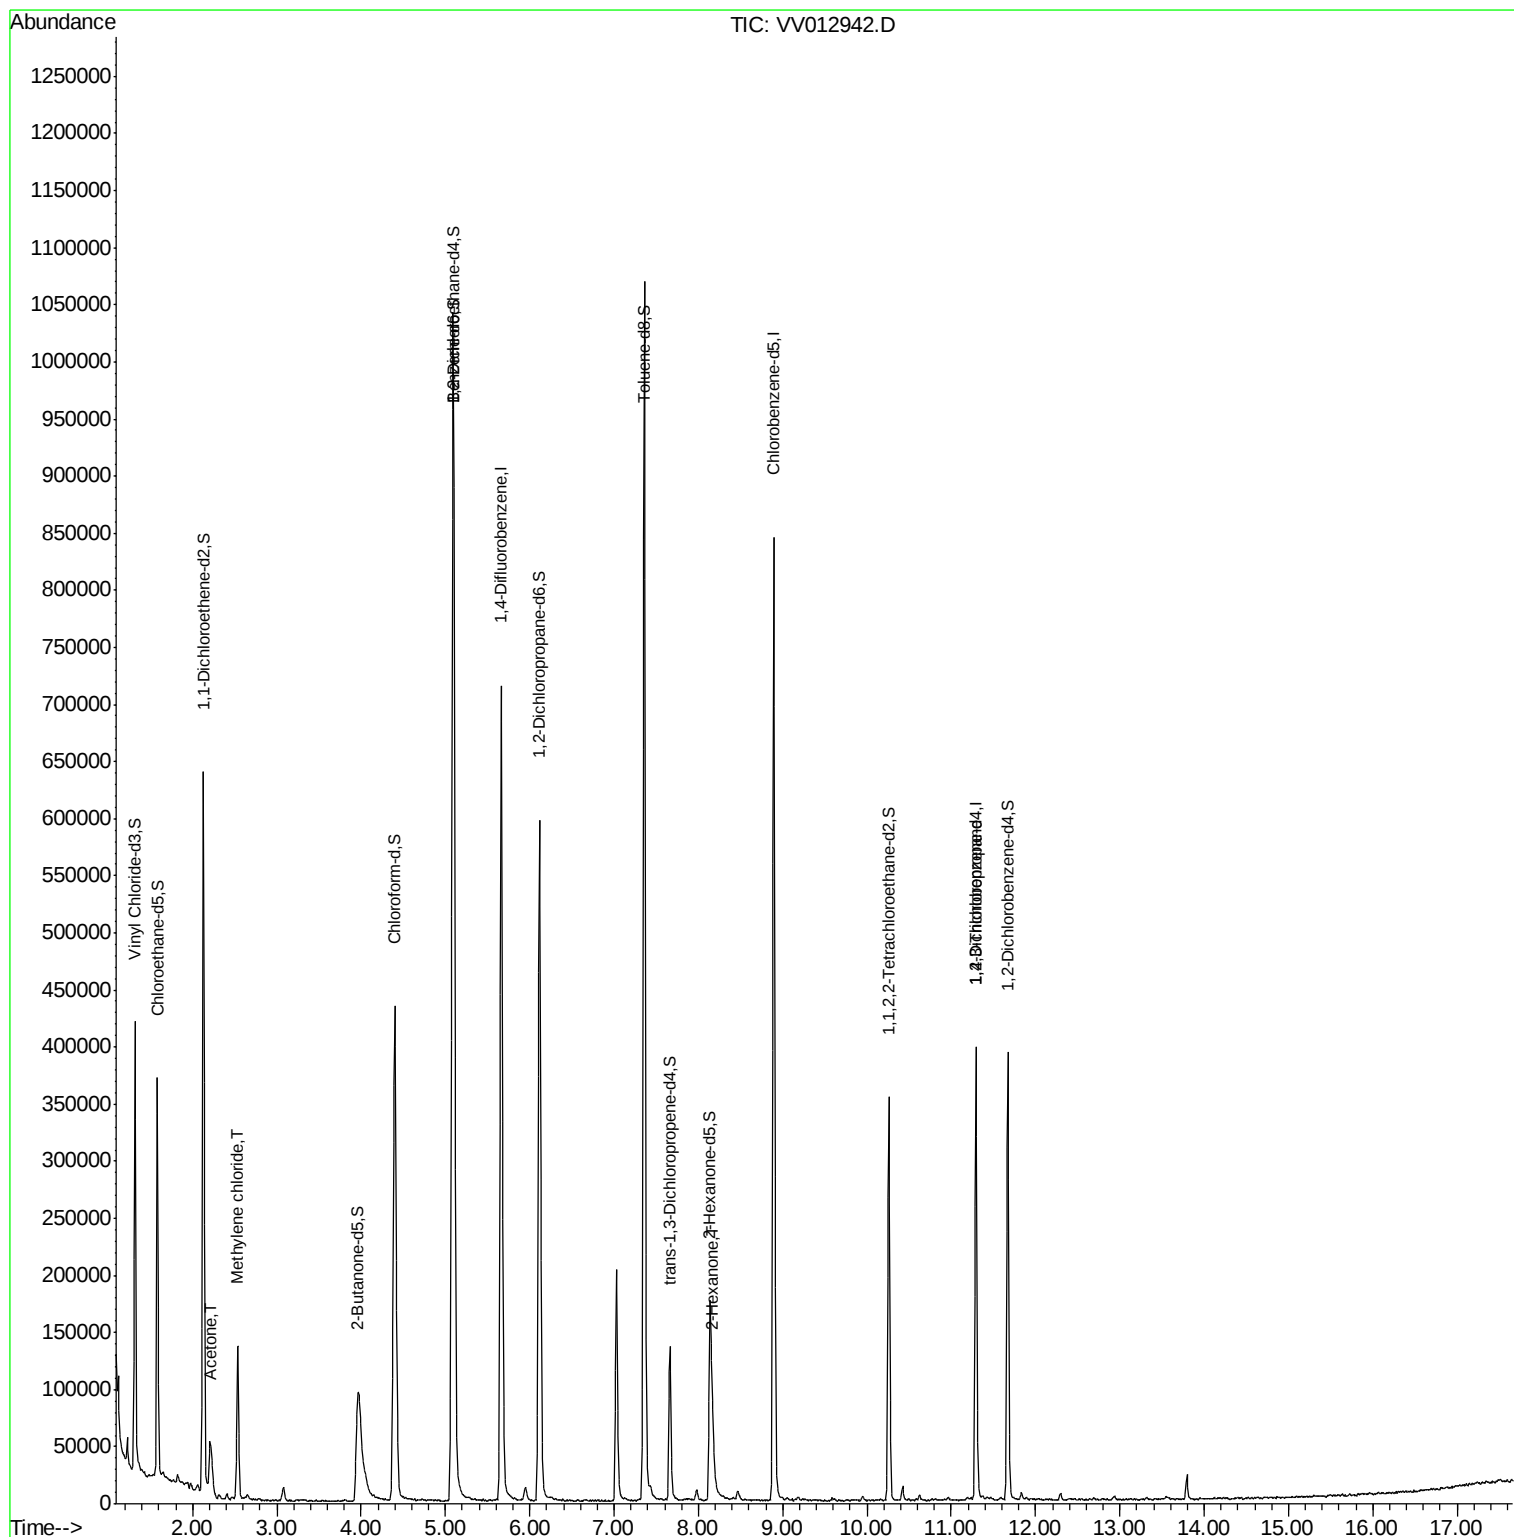

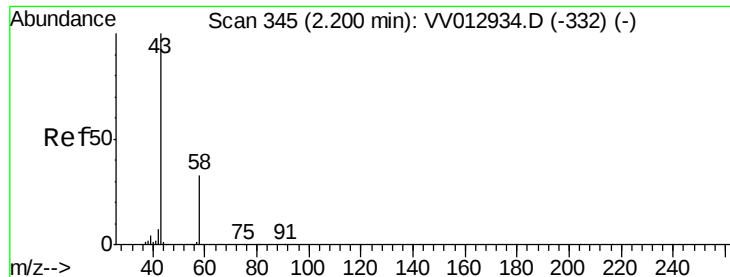

#13

Acetone

Concen: 19.726 ug/L

RT: 2.21 min Scan# 348

Delta R.T. 0.01 min

Lab File: VV012942.D

Acq: 23 Sep 2019 17:49

Instrument :

MSVOA_V

ClientSampleId :





ESNY4

Tgt Ion: 43 Resp: 68851

Ion Ratio Lower Upper

43 100

58 32.5 0.0 65.0

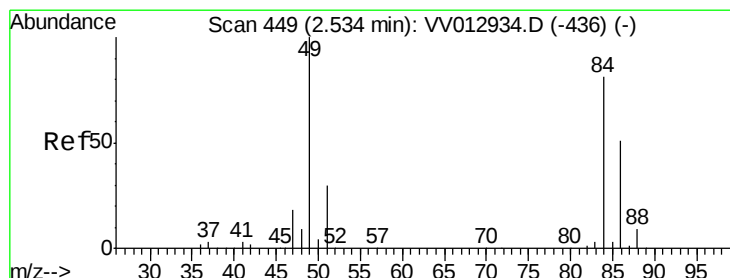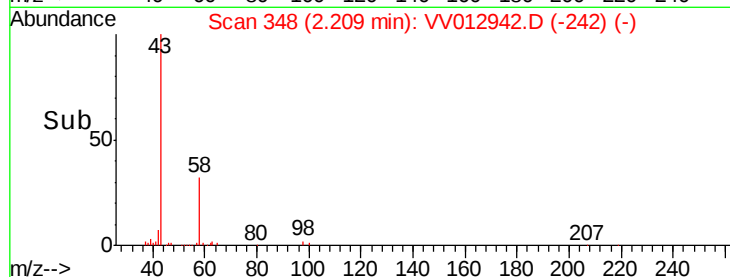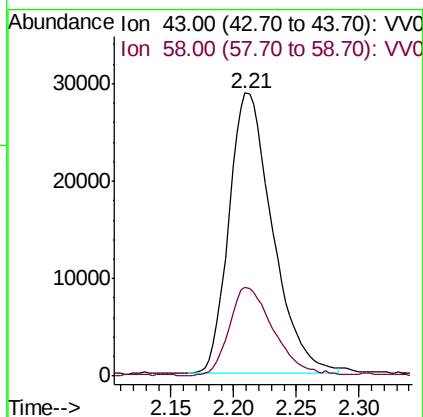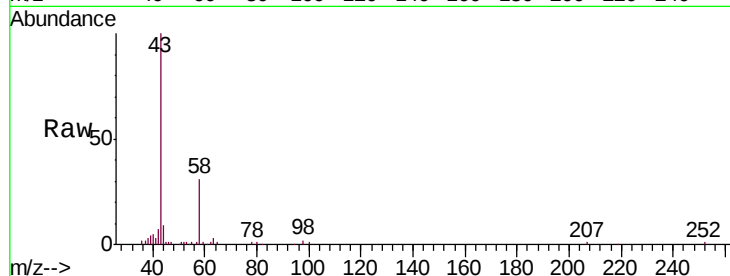

#16

Methylene chloride

Concen: 5.868 ug/L

RT: 2.54 min Scan# 450

Delta R.T. 0.00 min

Lab File: VV012942.D

Acq: 23 Sep 2019 17:49




Tgt Ion: 84 Resp: 53759


Ion Ratio Lower Upper

84 100

49 124.5 88.3 164.1

86 62.9 44.9 83.3

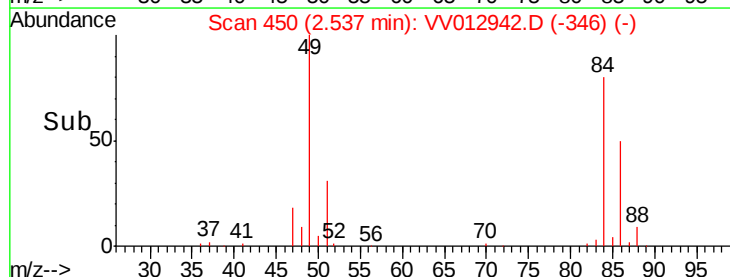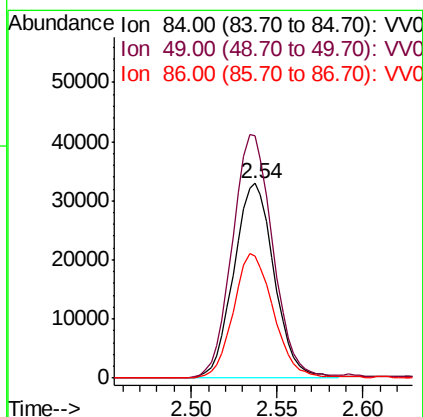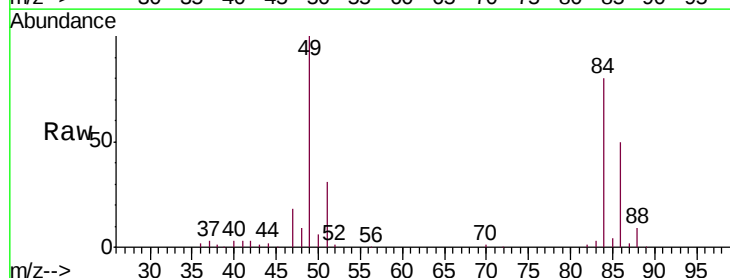

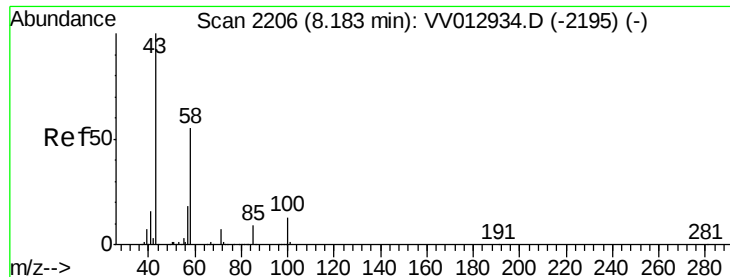

#49

2-Hexanone

Concen: 8.902 ug/L

RT: 8.17 min Scan# 2203

Delta R.T. -0.01 min

Lab File: VV012942.D

Acq: 23 Sep 2019 17:49

Instrument :

MSVOA_V

ClientSampleId :

ESNY4

Tgt Ion: 43 Resp: 37154


Ion Ratio Lower Upper

43 100

58 0.0 46.5 69.7#

57 0.0 15.5 23.3#

100 0.5 9.7 14.5#



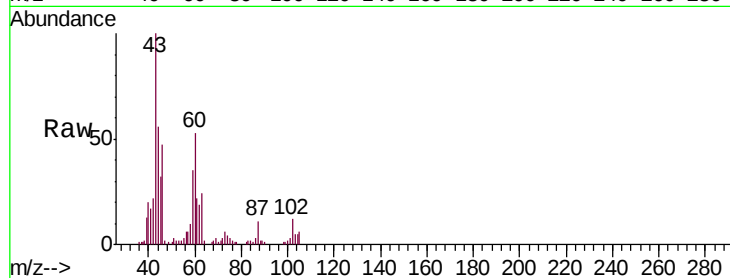


Abundance Ion 43.00 (42.70 to 43.70): VV012934.D (-2195) (-)

Ion 58.00 (57.70 to 58.70): VV012934.D (-2195) (-)

Ion 57.00 (56.70 to 57.70): VV012934.D (-2195) (-)

Ion 100.00 (99.70 to 100.70): VV012934.D (-2195) (-)

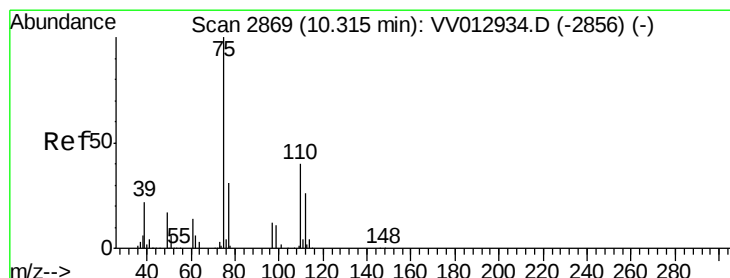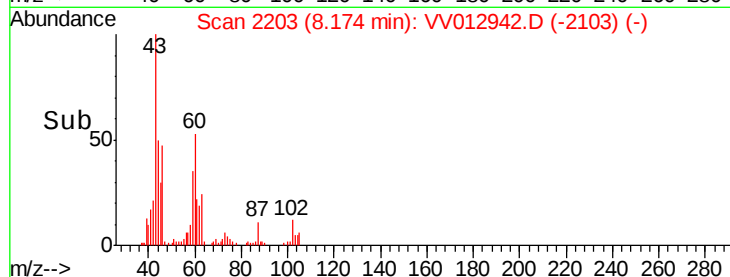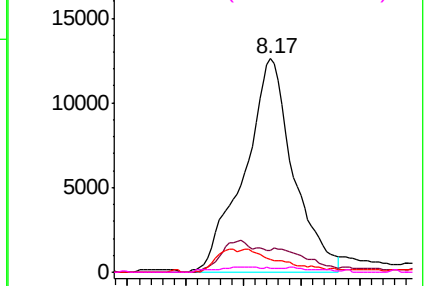

#59

1,2,3-Trichloropropane

Concen: 2.175 ug/L

RT: 11.29 min Scan# 3173

Delta R.T. 0.98 min

Lab File: VV012942.D


Acq: 23 Sep 2019 17:49

Tgt Ion: 75 Resp: 12708

Ion Ratio Lower Upper

75 100

77 32.1 25.4 38.0

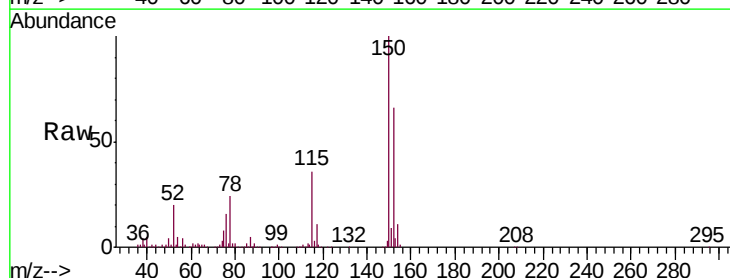

Abundance Ion 75.00 (74.70 to 75.70): VV012934.D (-2856) (-)

Ion 77.00 (76.70 to 77.70): VV012934.D (-2856) (-)

