


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092319\
Data File : VV012927.D
Acq On : 23 Sep 2019 08:54
Operator : SY/MD
Sample : BFB61
Misc : 5.00G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB61

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Title : VOC Analysis
Last Update : Thu Sep 19 17:48:44 2019

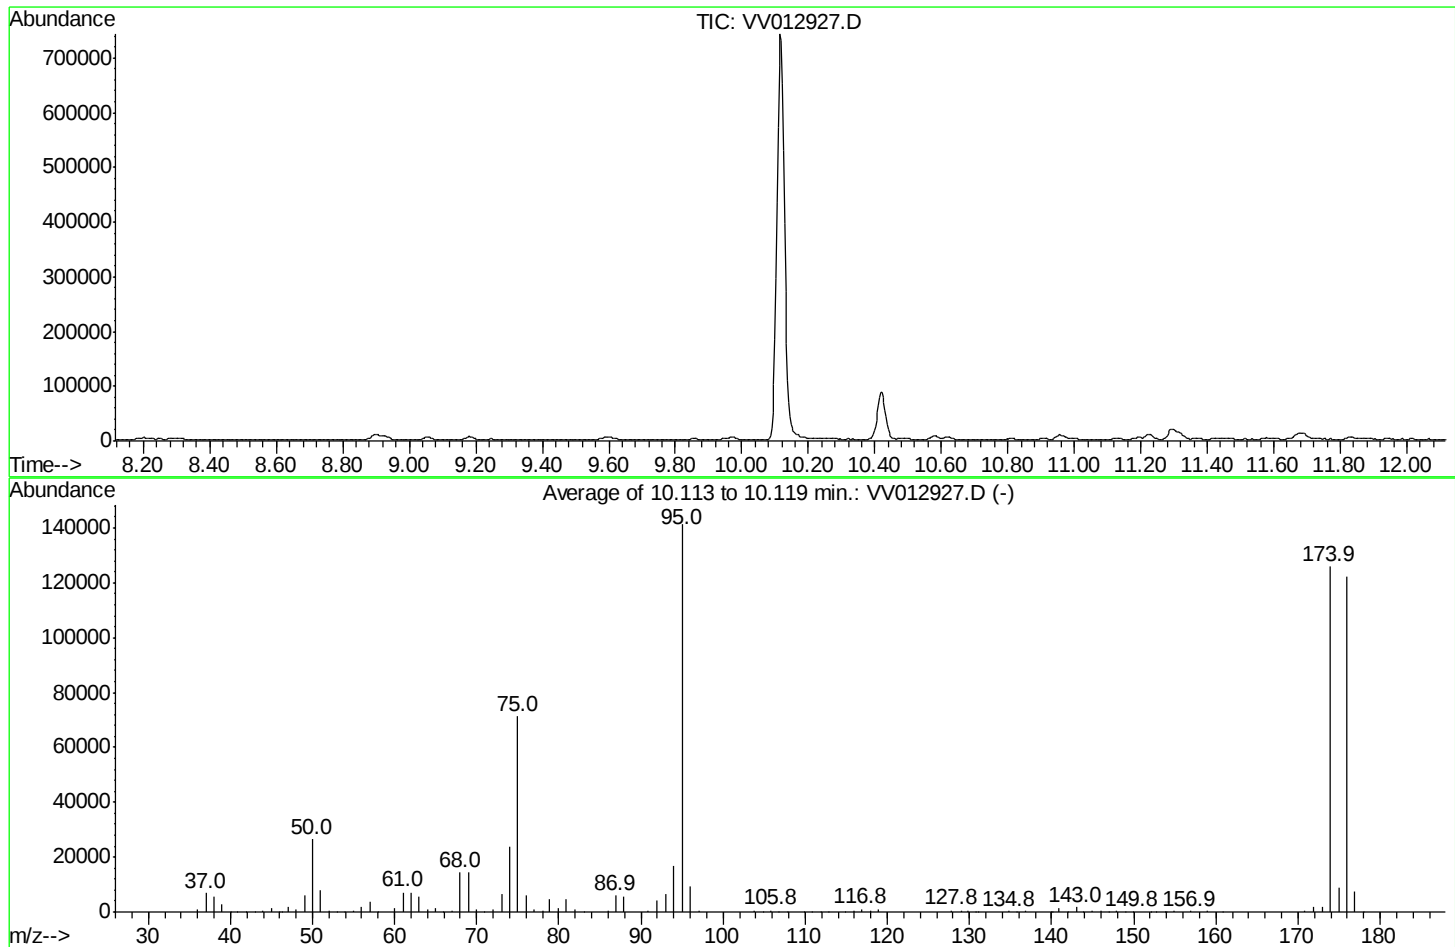

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	26522	PASS
75	95	30	80	50.4	71176	PASS
95	95	100	100	100.0	141290	PASS
96	95	5	9	6.6	9394	PASS
173	174	0.00	2	1.4	1714	PASS
174	95	50	120	89.1	125834	PASS
175	174	5	9	7.1	8974	PASS
176	174	95	101	97.2	122336	PASS
177	176	5	9	6.1	7517	PASS

m/z	Abundance
36.00	1233.0
37.00	6704.0
38.00	5548.0
39.00	2827.0
40.00	1305.0
42.00	147.0
43.00	200.0
44.00	1576.0
45.00	1204.0
46.00	287.0
47.10	1764.0
48.00	670.0
49.10	5778.0
50.00	25776.0
51.00	7819.0
52.00	538.0
52.90	152.0
53.90	101.0
55.00	421.0
56.00	1687.0
57.00	3533.0
57.90	165.0
60.00	1502.0
61.00	6976.0
62.00	6362.0
63.00	5641.0
64.00	1085.0
64.90	1231.0
65.90	157.0
67.00	456.0
68.00	13814.0
69.00	13948.0
70.00	913.0
70.80	156.0
72.00	792.0
73.00	6294.0
74.00	23024.0
75.00	68696.0
76.00	6031.0
77.00	728.0
78.00	695.0
78.90	4383.0
79.90	1211.0
80.90	4492.0
81.90	1141.0
83.00	131.0
86.00	236.0
86.90	5727.0
88.00	5547.0
90.90	585.0
92.00	4035.0
93.00	6182.0
94.00	15768.0
95.00	135104.0
96.00	9089.0
97.00	362.0
103.80	517.0
104.80	225.0
105.80	555.0
106.70	149.0
110.90	119.0
111.80	123.0
112.80	190.0
114.90	150.0
115.90	464.0
116.90	863.0
117.90	507.0
118.90	749.0
127.90	606.0
129.00	204.0
129.80	500.0
130.70	177.0
131.00	149.0
134.80	286.0
136.80	238.0
139.90	139.0
140.90	1391.0
142.00	147.0
143.00	1687.0
144.90	676.0
146.00	238.0
147.90	342.0
149.00	116.0
152.70	120.0
153.80	125.0
154.90	318.0
156.90	317.0
158.90	298.0
160.90	131.0
170.90	283.0
171.90	1542.0
173.00	1632.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

173.90	118080.0
174.90	8164.0
175.90	113600.0
177.00	7193.0
177.90	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
36.00	1253.0
37.00	7089.0
38.00	5995.0
39.00	3011.0
40.00	1363.0
41.90	125.0
43.00	199.0
44.00	1624.0
45.00	1370.0
46.20	294.0
47.10	1788.0
47.90	743.0
49.10	6311.0
50.00	27408.0
51.00	8352.0
52.00	513.0
52.90	176.0
53.90	120.0
55.00	391.0
56.00	1822.0
57.00	3778.0
57.90	163.0
60.00	1602.0
61.00	7479.0
62.00	7090.0
63.00	5970.0
64.00	1131.0
64.90	1380.0
66.00	135.0
67.00	495.0
68.00	14959.0
69.00	15059.0
70.00	882.0
70.90	158.0
72.00	800.0
73.00	6976.0
74.00	24560.0
75.00	73528.0
76.00	6304.0
77.00	825.0
78.00	743.0
78.90	4832.0
79.90	1358.0
80.90	4732.0
81.90	1187.0
83.00	125.0
86.00	271.0
86.90	6042.0
88.00	6020.0
90.90	618.0
92.00	4082.0
93.00	6783.0
94.00	17096.0
95.00	145536.0
96.00	9724.0
97.00	370.0
103.80	573.0
104.80	216.0
105.80	624.0
106.70	128.0
110.80	127.0
111.90	112.0
112.80	170.0
114.80	145.0
115.90	474.0
116.80	948.0
117.90	567.0
118.90	821.0
127.90	562.0
129.00	280.0
129.90	543.0
130.70	206.0
134.90	331.0
135.80	105.0
136.90	298.0
140.10	171.0
140.90	1445.0
142.00	132.0
143.00	1721.0
143.90	118.0
144.90	660.0
146.00	271.0
147.90	352.0
149.00	137.0
149.80	117.0
152.10	107.0
153.80	131.0
154.90	315.0
156.90	329.0
158.90	328.0
160.80	145.0
170.80	308.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

171.90	1737.0
173.00	1797.0
173.90	129824.0
175.00	9278.0
175.90	126528.0
177.00	7731.0
178.00	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

m/z	Abundance
36.00	1142.0
37.00	6689.0
38.00	5952.0
39.00	2747.0
40.00	1350.0
40.80	113.0
41.90	127.0
43.10	181.0
44.00	1548.0
45.00	1448.0
46.20	282.0
47.00	1589.0
47.90	807.0
49.00	5956.0
50.00	26384.0
51.00	8265.0
52.00	448.0
52.90	215.0
55.00	352.0
56.00	1875.0
57.00	3716.0
57.90	159.0
60.00	1515.0
61.00	7154.0
62.00	6979.0
63.00	5702.0
64.00	1010.0
65.00	1335.0
65.90	126.0
67.00	502.0
68.00	14231.0
69.00	14664.0
70.00	889.0
70.90	170.0
72.00	740.0
73.00	7073.0
74.00	23760.0
75.00	71304.0
76.00	6004.0
77.00	817.0
78.00	666.0
78.90	4823.0
80.00	1466.0
80.90	4638.0
81.90	1056.0
83.00	100.0
85.90	257.0
86.90	6075.0
87.90	5851.0
90.90	580.0
92.00	3897.0
93.00	6746.0
94.00	16936.0
95.00	143232.0
96.00	9370.0
97.00	341.0
103.90	622.0
104.80	203.0
105.90	671.0
106.80	107.0
107.80	116.0
109.90	118.0
110.80	131.0
112.80	124.0
114.80	144.0
115.90	501.0
116.80	1017.0
118.00	523.0
118.80	853.0
127.80	520.0
129.00	307.0
129.90	517.0
130.70	176.0
134.90	289.0
136.90	331.0
140.10	167.0
140.90	1319.0
141.90	115.0
143.00	1626.0
143.90	140.0
144.90	542.0
145.90	291.0
146.90	127.0
147.90	311.0
149.00	133.0
149.90	149.0
154.00	119.0
154.90	298.0
156.90	309.0
158.90	313.0
160.70	174.0
170.90	303.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

171.90	1810.0
173.00	1713.0
173.90	129600.0
175.00	9481.0
175.90	126880.0
176.90	7629.0
178.00	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61

Scan 2794 (10.074 min): VV012927.D
BFB61

m/z	Abundance
36.00	137.0
38.30	109.0
39.20	125.0
39.90	1272.0
41.20	126.0
42.90	113.0
43.90	930.0
55.00	131.0
63.30	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB61