


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV092320\
Data File : VV018402.D
Acq On : 23 Sep 2020 09:40
Operator : SY/MD
Sample : BFB97
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB301

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM092320W.M
Title : VOC Analysis
Last Update : Thu Sep 24 07:48:50 2020

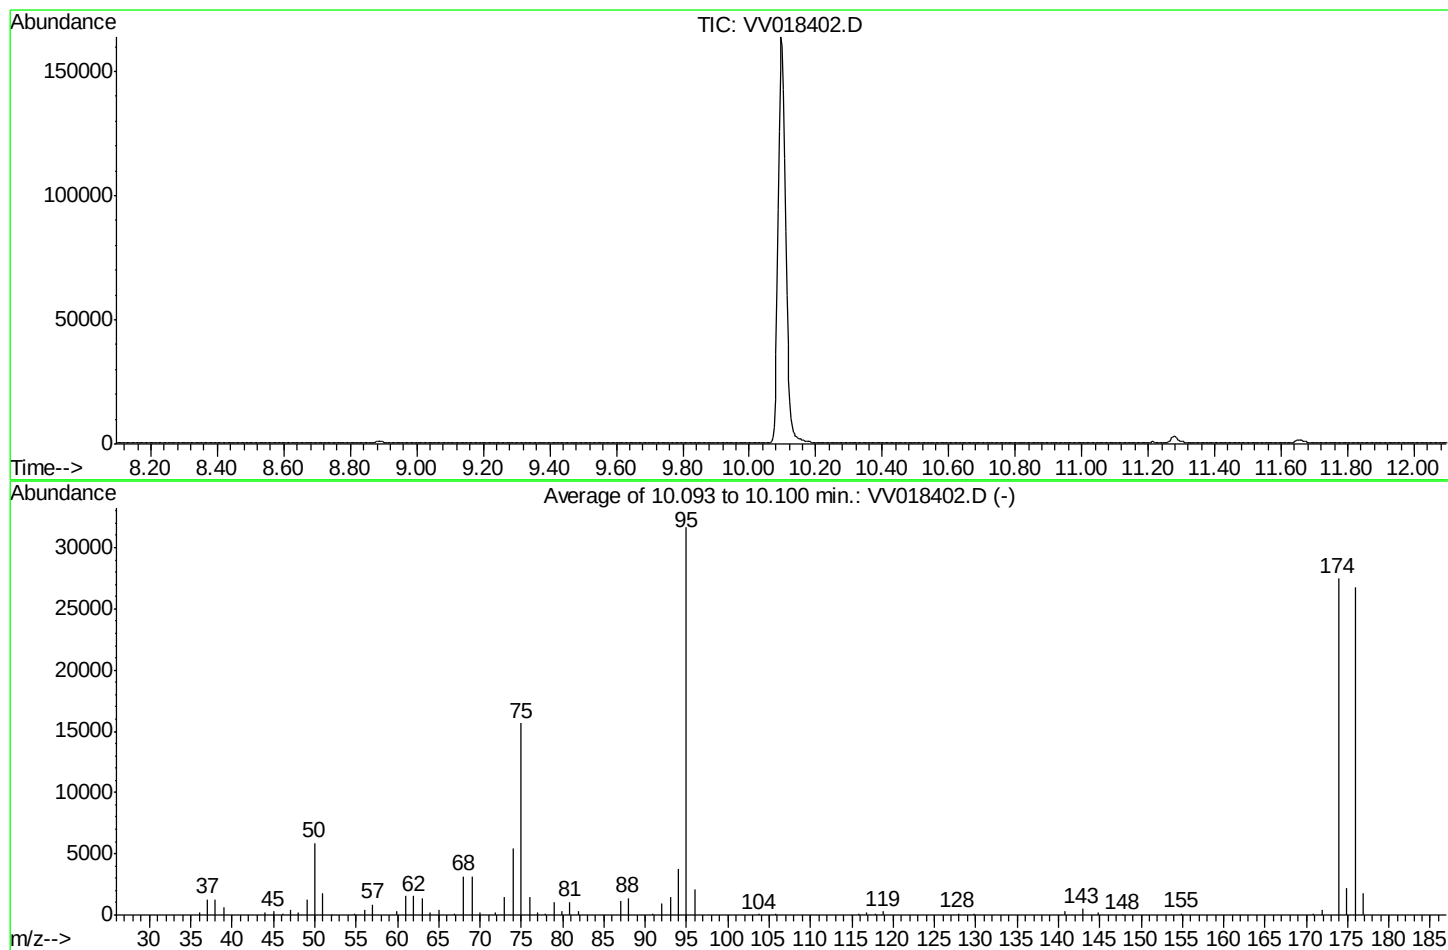

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	5902	PASS
75	95	30	80	49.4	15637	PASS
95	95	100	100	100.0	31653	PASS
96	95	5	9	6.5	2065	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.8	27464	PASS
175	174	5	9	8.1	2224	PASS
176	174	95	101	97.6	26805	PASS
177	176	5	9	6.8	1832	PASS

m/z	Abundance
36.00	252.0
37.00	1298.0
38.00	1216.0
39.00	622.0
39.80	172.0
44.00	441.0
45.00	270.0
47.00	426.0
48.00	217.0
49.00	1238.0
50.00	5768.0
51.00	1738.0
52.00	102.0
56.00	427.0
57.00	811.0
59.90	303.0
61.00	1526.0
62.00	1566.0
63.00	1330.0
63.90	231.0
65.00	431.0
67.00	120.0
68.00	3022.0
69.00	3039.0
70.00	237.0
71.90	167.0
73.00	1478.0
74.00	5289.0
75.00	15158.0
76.00	1530.0
76.90	240.0
77.90	177.0
78.90	1046.0
79.90	264.0
80.90	1043.0
81.90	253.0
87.00	1110.0
87.90	1411.0
90.80	123.0
92.00	854.0
93.00	1359.0
94.00	3516.0
95.00	30000.0
96.00	2127.0
103.80	146.0
115.80	115.0
116.80	222.0
118.80	228.0
127.90	125.0
129.90	139.0
140.90	338.0
142.90	449.0
144.80	156.0
154.90	114.0
170.90	100.0
172.00	392.0
173.90	25632.0
174.90	2082.0
175.90	25064.0
177.00	1765.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

m/z	Abundance
36.00	254.0
37.00	1311.0
38.00	1274.0
39.00	635.0
39.90	158.0
44.00	507.0
45.00	294.0
46.10	107.0
47.00	439.0
48.00	231.0
49.00	1312.0
50.00	6069.0
51.00	1816.0
54.80	106.0
56.00	455.0
57.00	871.0
59.90	314.0
61.00	1622.0
62.00	1612.0
63.00	1361.0
63.90	238.0
65.00	473.0
66.90	130.0
68.00	3332.0
69.00	3177.0
70.00	259.0
71.90	159.0
73.00	1515.0
74.00	5608.0
75.00	16172.0
76.00	1543.0
76.90	264.0
77.80	165.0
78.90	1129.0
80.00	273.0
80.90	1097.0
81.90	274.0
87.00	1191.0
87.90	1463.0
90.90	123.0
92.00	968.0
93.00	1502.0
94.00	3850.0
95.00	32752.0
96.00	2076.0
103.80	117.0
105.80	107.0
115.80	111.0
116.80	249.0
117.90	110.0
118.80	300.0
127.90	149.0
129.90	143.0
140.80	351.0
142.90	491.0
144.80	173.0
154.90	124.0
170.90	120.0
172.00	466.0
173.90	28392.0
174.90	2342.0
175.90	27752.0
177.00	1914.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

m/z	Abundance
36.00	238.0
37.00	1235.0
38.00	1277.0
39.00	590.0
39.90	158.0
44.00	559.0
45.00	274.0
46.10	127.0
47.00	422.0
48.00	244.0
49.00	1315.0
50.00	5871.0
51.00	1751.0
54.90	102.0
56.00	423.0
57.00	850.0
59.90	296.0
61.00	1498.0
62.00	1511.0
63.00	1289.0
63.90	232.0
65.00	409.0
66.90	119.0
68.00	3209.0
69.00	3054.0
70.00	277.0
71.90	162.0
73.00	1387.0
74.00	5386.0
75.00	15582.0
76.00	1425.0
77.00	252.0
78.90	1074.0
80.00	281.0
80.90	1063.0
81.90	286.0
87.00	1241.0
87.90	1281.0
91.00	125.0
92.00	1003.0
93.00	1539.0
94.00	3831.0
95.00	32208.0
96.00	1994.0
105.80	116.0
116.80	230.0
117.90	140.0
118.80	329.0
127.90	158.0
129.80	125.0
140.80	355.0
142.90	528.0
144.80	196.0
147.80	118.0
154.90	103.0
170.80	116.0
171.90	511.0
173.90	28368.0
174.90	2249.0
175.90	27600.0
176.90	1818.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301

Scan 2790 (10.061 min): VV018402.D
BFB97

m/z	Abundance
39.90	165.0
44.00	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB301