

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V092321\
 Data File : VV022295.D
 Acq On : 23 Sep 2021 19:45
 Operator : SY/MD
 Sample : M3873-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7Y6

Manual Integrations
 APPROVED

MMDadoda
 9/27/2021 10:55:15 AM

Quant Time: Sep 24 03:46:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 03:31:01 2021
 Response via : Initial Calibration

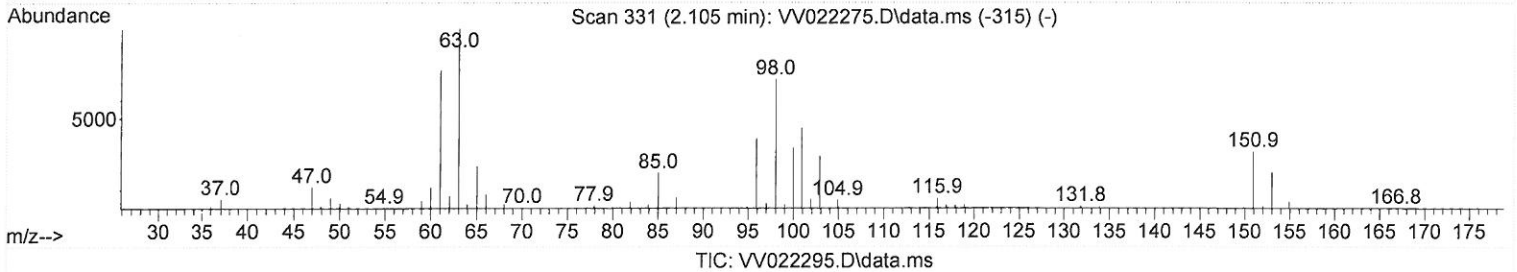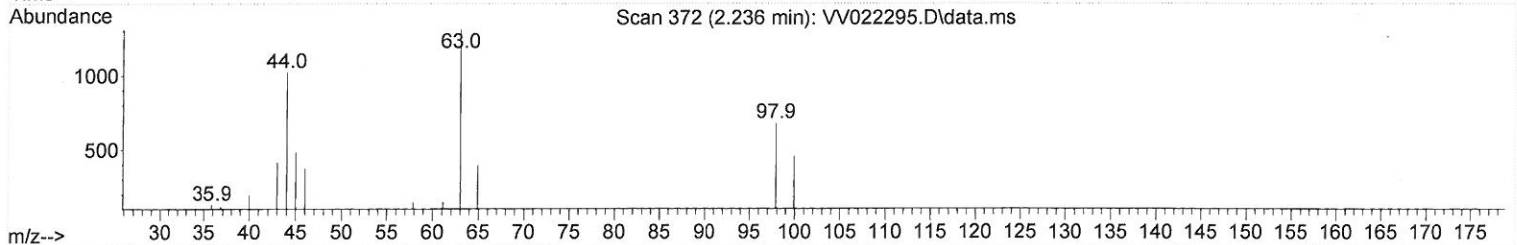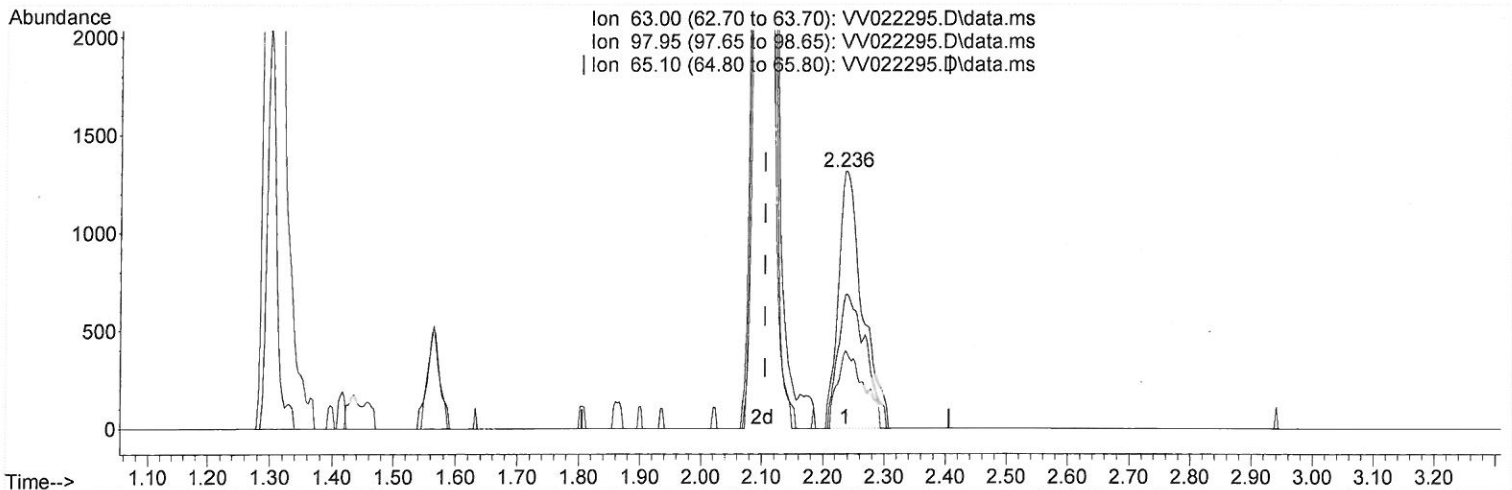

(11) 1,1-Dichloroethene-d2 (S)

2.236min (+ 0.131) 0.25 ug/L

response 3607

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	74.30	60.49
65.10	22.80	27.83
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022295.D
Acq On : 23 Sep 2021 19:45
Operator : SY/MD
Sample : M3873-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7Y6

Manual Integrations
APPROVED

MMDadoda
9/27/2021 10:55:15 AM

Quant Time: Sep 24 03:46:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 24 03:31:01 2021
Response via : Initial Calibration

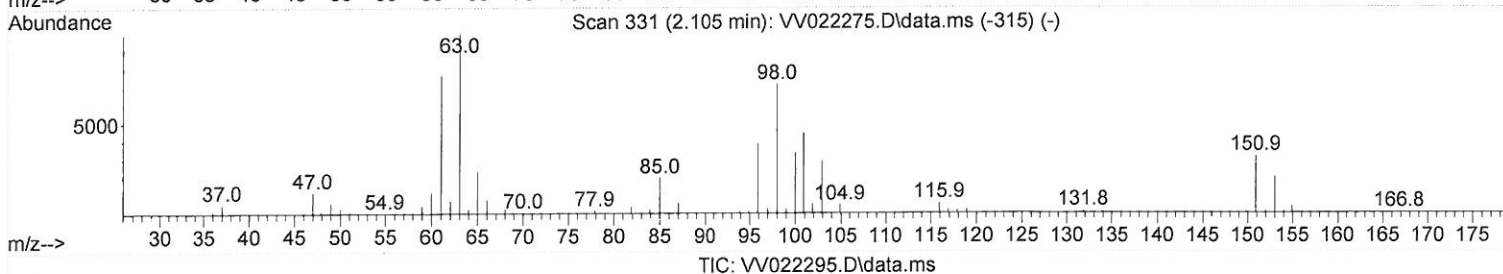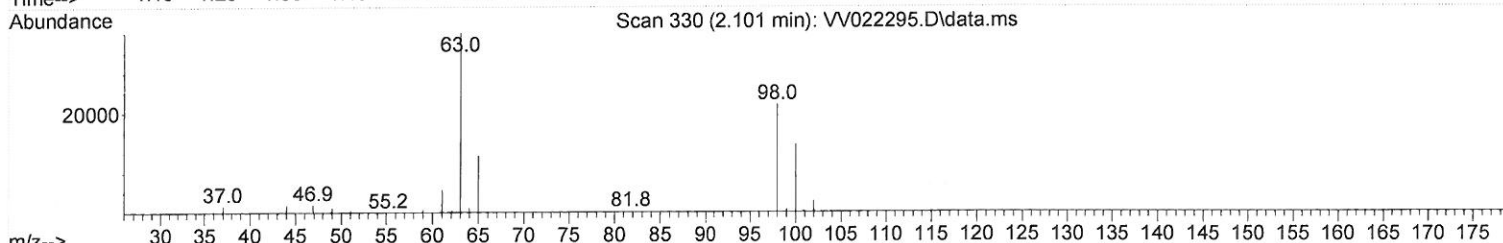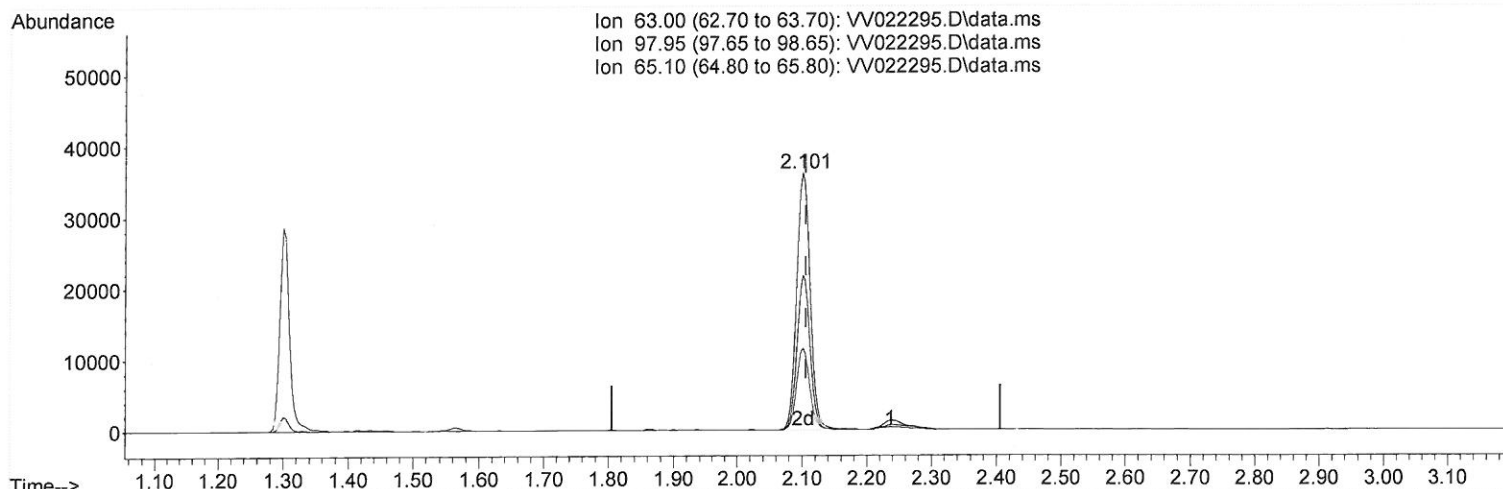

(11) 1,1-Dichloroethene-d2 (S)

2.101min (-0.004) 3.64 ug/L m

response 52264

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	74.30	4.17#
65.10	22.80	1.92#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022295.D
 Acq On : 23 Sep 2021 19:45
 Operator : SY/MD
 Sample : M3873-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7Y6

Manual Integrations
 APPROVED

MMDadoda
 9/27/2021 10:55:15 AM

Quant Time: Sep 24 03:46:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 03:31:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	119442	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	118468	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	51600	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	29664	4.929	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	98.600%	
7) Chloroethane-d5	1.564	69	36434	5.173	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	103.400%	
11) 1,1-Dichloroethene-d2	2.101	63	52264m	3.642	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.800%	
20) 2-Butanone-d5	3.908	46	132267	53.778	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	107.560%	
24) Chloroform-d	4.352	84	85607	4.959	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.200%	
26) 1,2-Dichloroethane-d4	5.037	65	43057	5.221	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.400%	
32) Benzene-d6	5.050	84	170339	5.113	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.200%	
36) 1,2-Dichloropropane-d6	6.072	67	55523	5.337	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.800%	
41) Toluene-d8	7.316	98	144057	4.789	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.800%	
43) trans-1,3-Dichloroprop...	7.628	79	14355	4.518	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.400%	
46) 2-Hexanone-d5	8.091	63	108395	54.867	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	109.740%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	44457	5.076	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.600%	
66) 1,2-Dichlorobenzene-d4	11.628	152	54984	5.678	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	113.600%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022295.D
Acq On : 23 Sep 2021 19:45
Operator : SY/MD
Sample : M3873-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7Y6

Manual Integrations
APPROVED

MMDadoda
9/27/2021 10:55:15 AM

Quant Time: Sep 24 03:46:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 24 03:31:01 2021
Response via : Initial Calibration

