

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022300.D
 Acq On : 23 Sep 2021 22:11
 Operator : SY/MD
 Sample : M3878-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2N8

Manual Integrations
 APPROVED

MMDadoda
 9/27/2021 10:55:19 AM

Quant Time: Sep 24 05:11:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 05:07:58 2021
 Response via : Initial Calibration

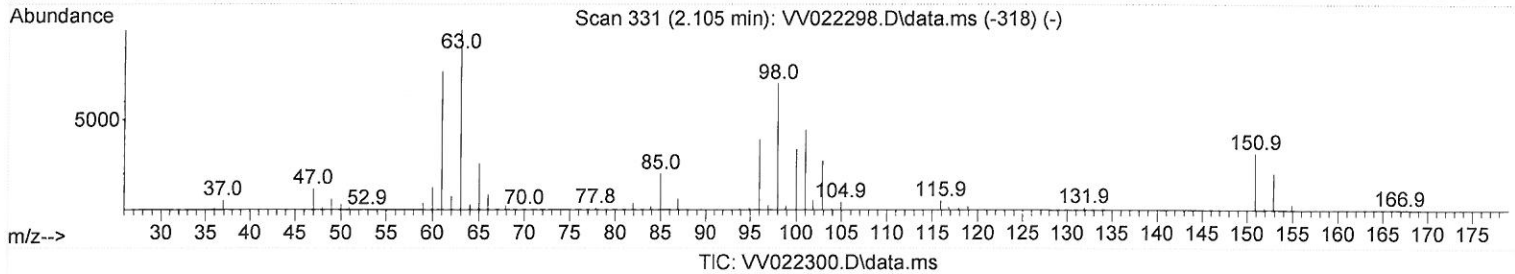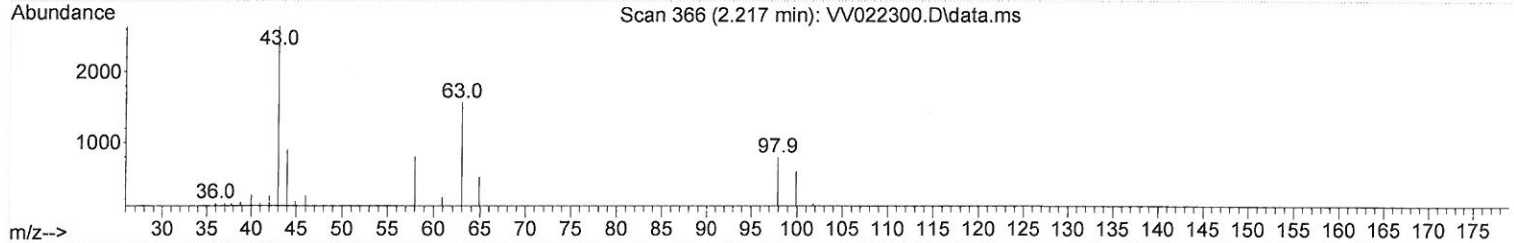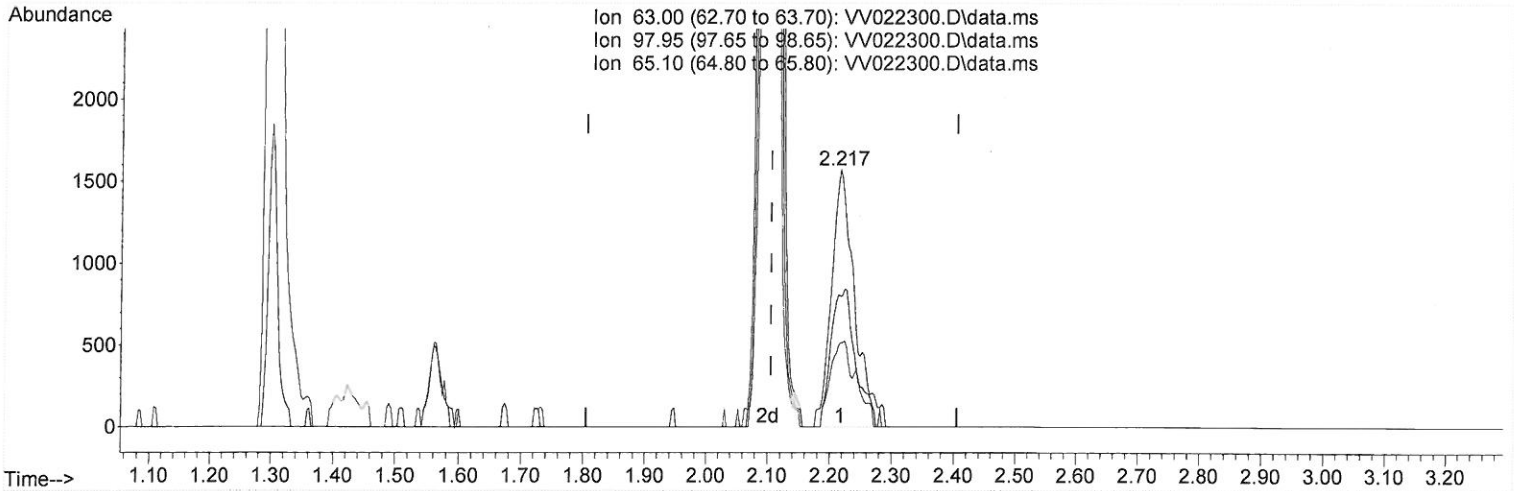

(11) 1,1-Dichloroethene-d2 (S)

2.217min (+ 0.112) 0.28 ug/L

response 4134

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	74.30	56.22
65.10	22.80	27.33
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022300.D
 Acq On : 23 Sep 2021 22:11
 Operator : SY/MD
 Sample : M3878-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2N8

Manual Integrations
 APPROVED

MMDadoda
 9/27/2021 10:55:19 AM

Quant Time: Sep 24 05:11:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 05:07:58 2021
 Response via : Initial Calibration

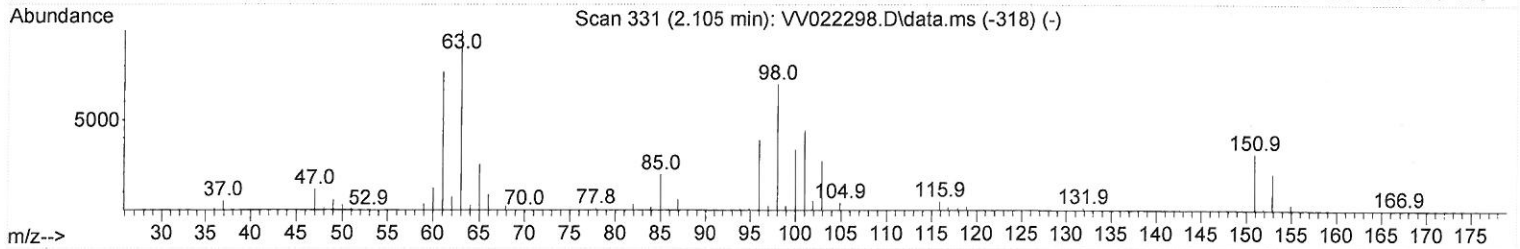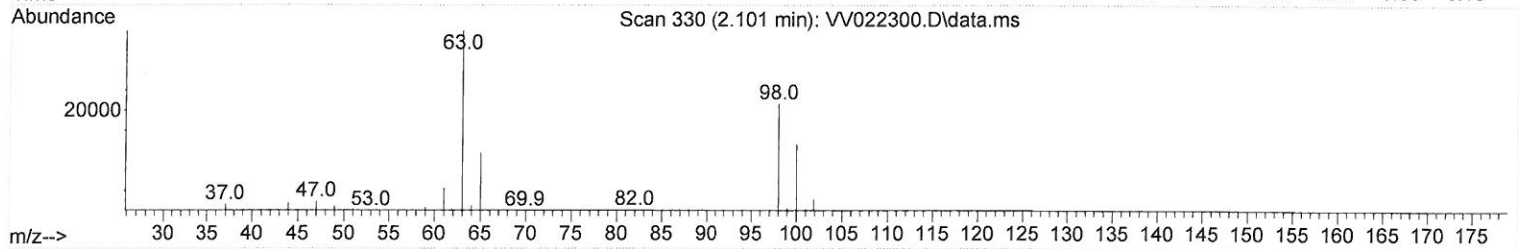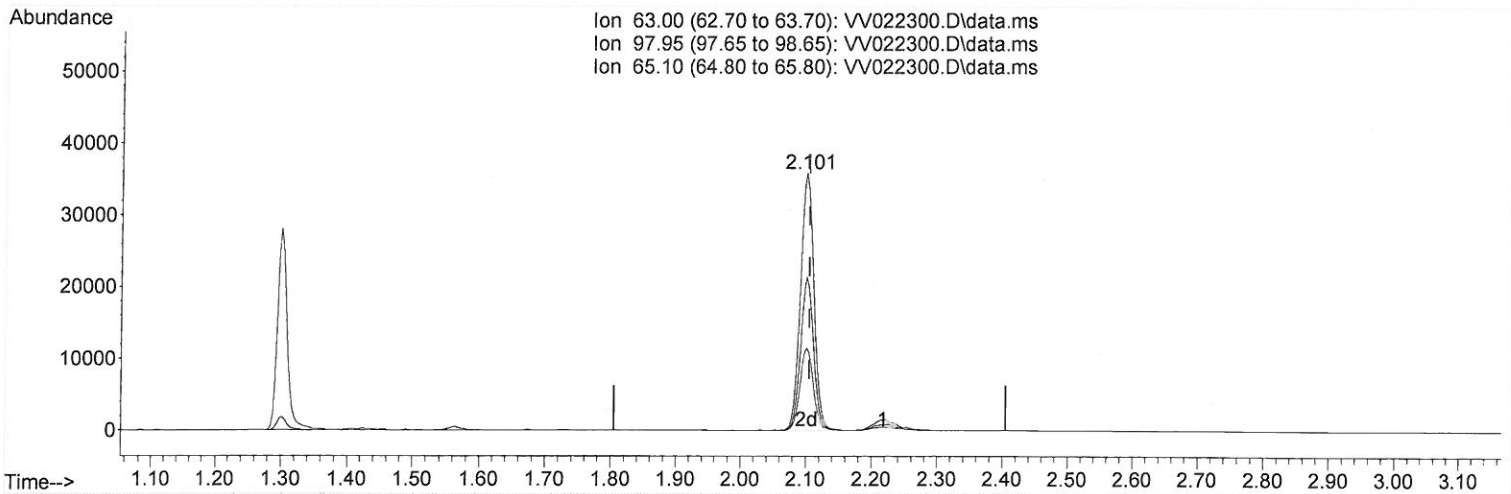

TIC: VV022300.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.101min (-0.003) 3.46 ug/L m

response 51098

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	74.30	4.55#
65.10	22.80	2.21#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022300.D
 Acq On : 23 Sep 2021 22:11
 Operator : SY/MD
 Sample : M3878-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2N8

Manual Integrations
 APPROVED

MMDadoda
 9/27/2021 10:55:19 AM

Quant Time: Sep 24 05:11:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 05:07:58 2021
 Response via : Initial Calibration

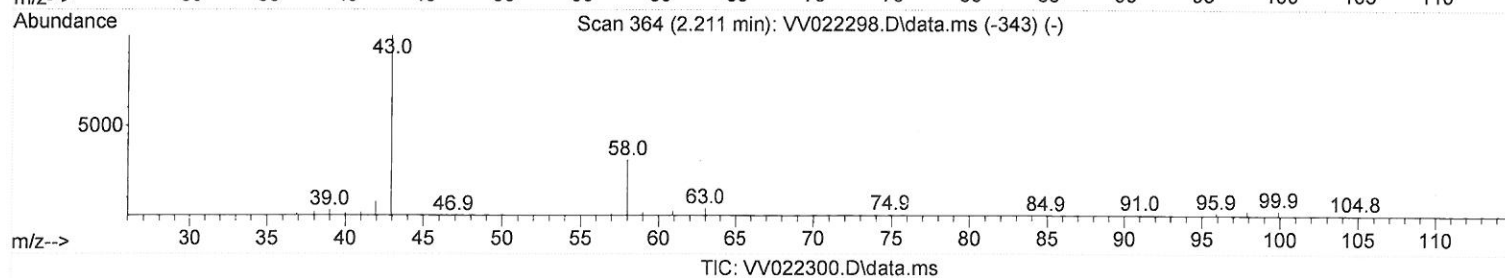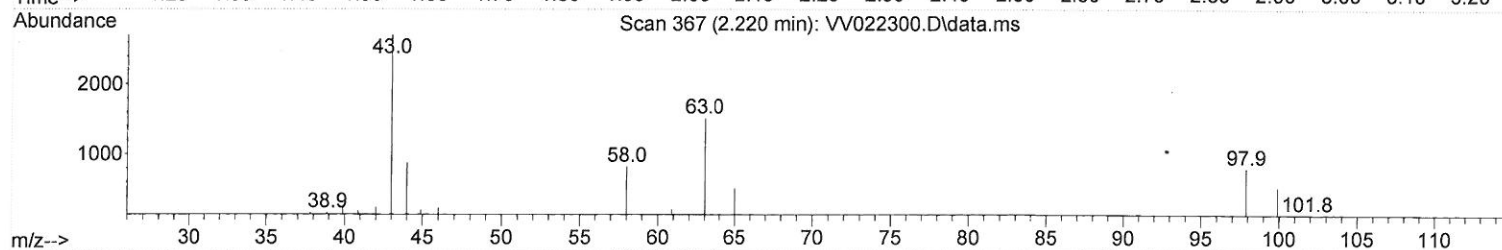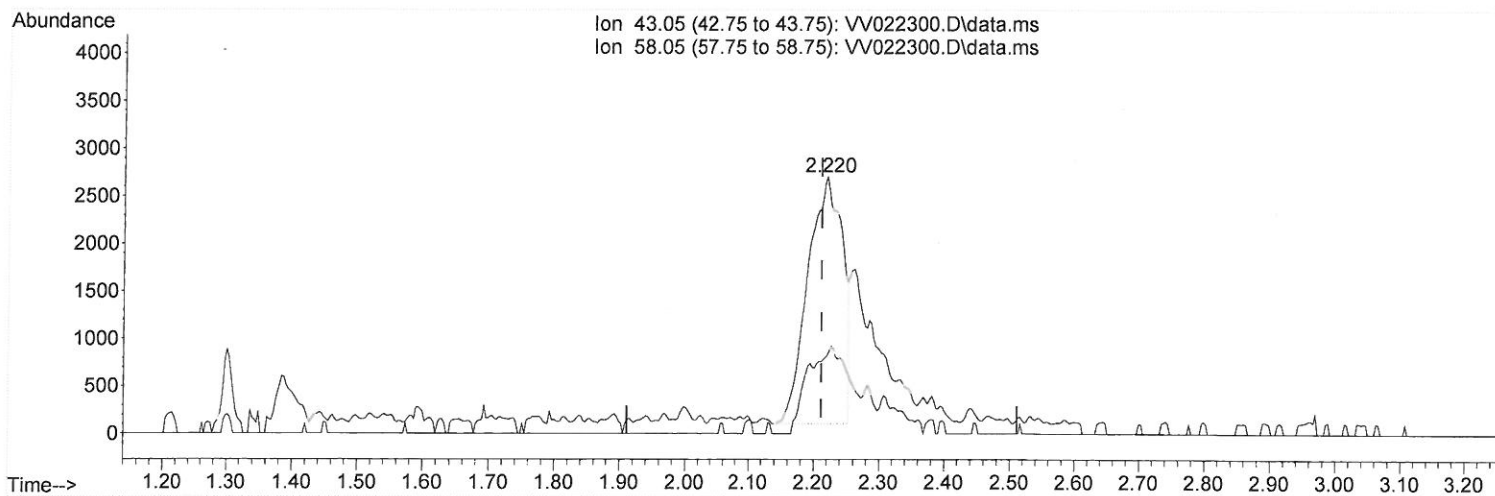

TIC: VV022300.D\data.ms

(13) Acetone (T)

2.220min (+ 0.009) 6.65 ug/L

response 9542

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.10	23.21
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022300.D
 Acq On : 23 Sep 2021 22:11
 Operator : SY/MD
 Sample : M3878-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2N8

Manual Integrations
 APPROVED

MMDadoda
 9/27/2021 10:55:19 AM

Quant Time: Sep 24 05:11:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 05:07:58 2021
 Response via : Initial Calibration

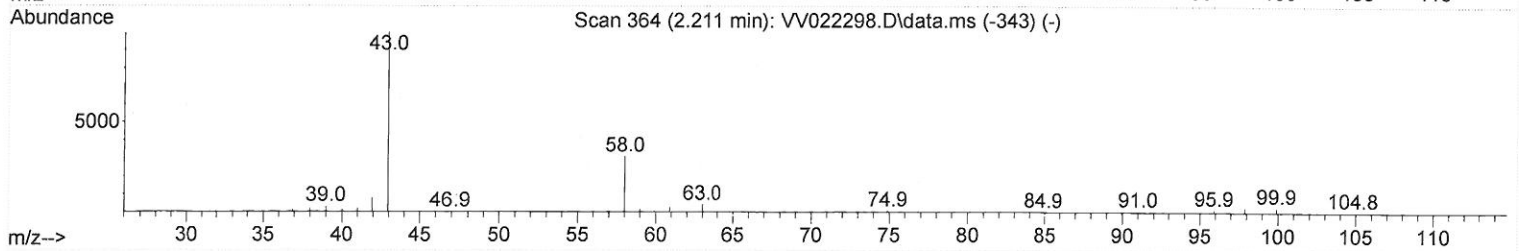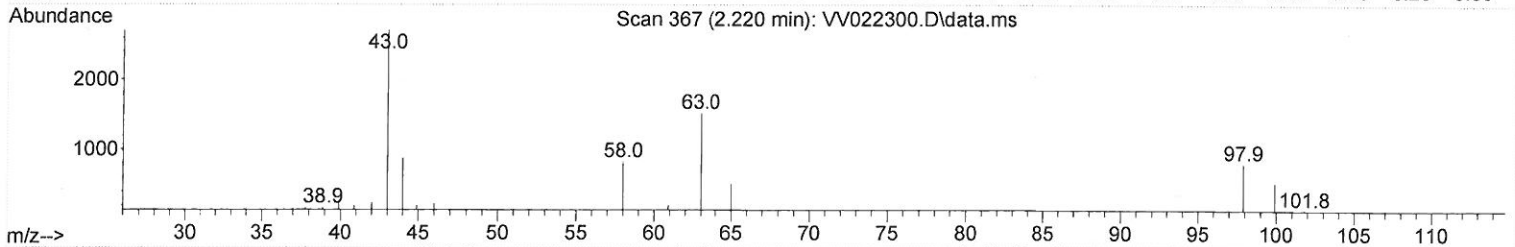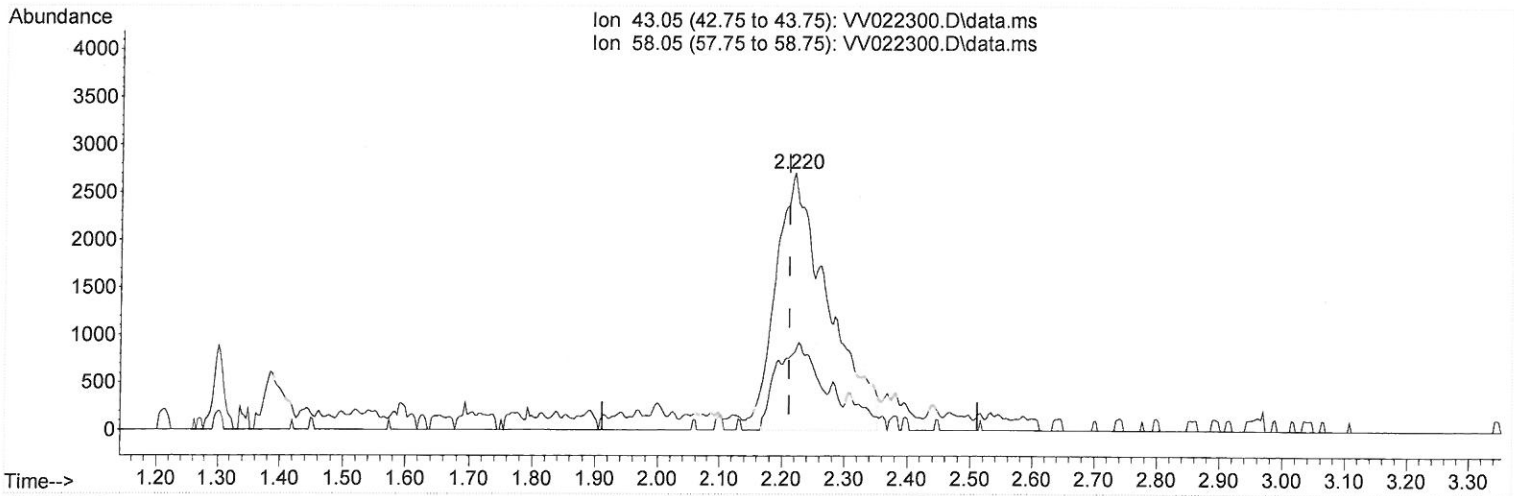

TIC: VV022300.D\data.ms

(13) Acetone (T)

2.220min (+ 0.009) 10.97 ug/L m >10/01/21 EQ

response 15738

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.10	14.07
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW092321\
 Data File : VW022300.D
 Acq On : 23 Sep 2021 22:11
 Operator : SY/MD
 Sample : M3878-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2N8

Manual Integrations
 APPROVED

MMDadoda
 9/27/2021 10:55:19 AM

Quant Time: Sep 24 05:11:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 05:07:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	122862	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	123485	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	53572	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	28436	4.593	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	91.800%	
7) Chloroethane-d5	1.561	69	35706	4.928	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	98.600%	
11) 1,1-Dichloroethene-d2	2.101	63	51098m	3.462	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	69.200%	
20) 2-Butanone-d5	3.918	46	118942	47.014	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	94.020%	
24) Chloroform-d	4.349	84	83799	4.719	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.400%	
26) 1,2-Dichloroethane-d4	5.037	65	42154	4.969	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.400%	
32) Benzene-d6	5.050	84	169115	4.870	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.400%	
36) 1,2-Dichloropropane-d6	6.069	67	56215	5.184	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	103.600%	
41) Toluene-d8	7.317	98	141128	4.501	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.000%	
43) trans-1,3-Dichloroprop...	7.628	79	14533	4.388	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.800%	
46) 2-Hexanone-d5	8.095	63	103268	50.148	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	100.300%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	40422	4.428	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	88.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	53749	5.346	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	107.000%	
Target Compounds						
13) Acetone	2.220	43	15738m	10.972	ug/L	Qvalue 88
42) Toluene	7.397	91	3935	0.114	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022300.D
Acq On : 23 Sep 2021 22:11
Operator : SY/MD
Sample : M3878-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2N8

Manual Integrations
APPROVED

MMDadoda
9/27/2021 10:55:19 AM

Quant Time: Sep 24 05:11:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 24 05:07:58 2021
Response via : Initial Calibration

