

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022279.D
 Acq On : 23 Sep 2021 13:15
 Operator : SY/MD
 Sample : VV0923WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK209

Quant Time: Sep 24 03:44:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 03:31:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	133005	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	129321	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	58151	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	33156	4.947	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	99.000%
7) Chloroethane-d5	1.561	69	39205	4.999	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.000%
11) 1,1-Dichloroethene-d2	2.101	63	58734	3.676	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.600%
20) 2-Butanone-d5	3.908	46	133550	48.763	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.520%
24) Chloroform-d	4.349	84	90772	4.722	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.400%
26) 1,2-Dichloroethane-d4	5.034	65	46636	5.078	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
32) Benzene-d6	5.050	84	190247	5.232	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.600%
36) 1,2-Dichloropropane-d6	6.069	67	59215	5.214	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.200%
41) Toluene-d8	7.317	98	157379	4.792	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.800%
43) trans-1,3-Dichloroprop...	7.625	79	15622	4.504	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.000%
46) 2-Hexanone-d5	8.091	63	110963	51.454	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.900%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	45729	4.783	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.600%
66) 1,2-Dichlorobenzene-d4	11.628	152	59011	5.407	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.200%
Target Compounds					Qvalue	
42) Toluene	7.394	91	3378	0.094	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022279.D
Acq On : 23 Sep 2021 13:15
Operator : SY/MD
Sample : VV0923WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK209

Quant Time: Sep 24 03:44:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 24 03:31:01 2021
Response via : Initial Calibration

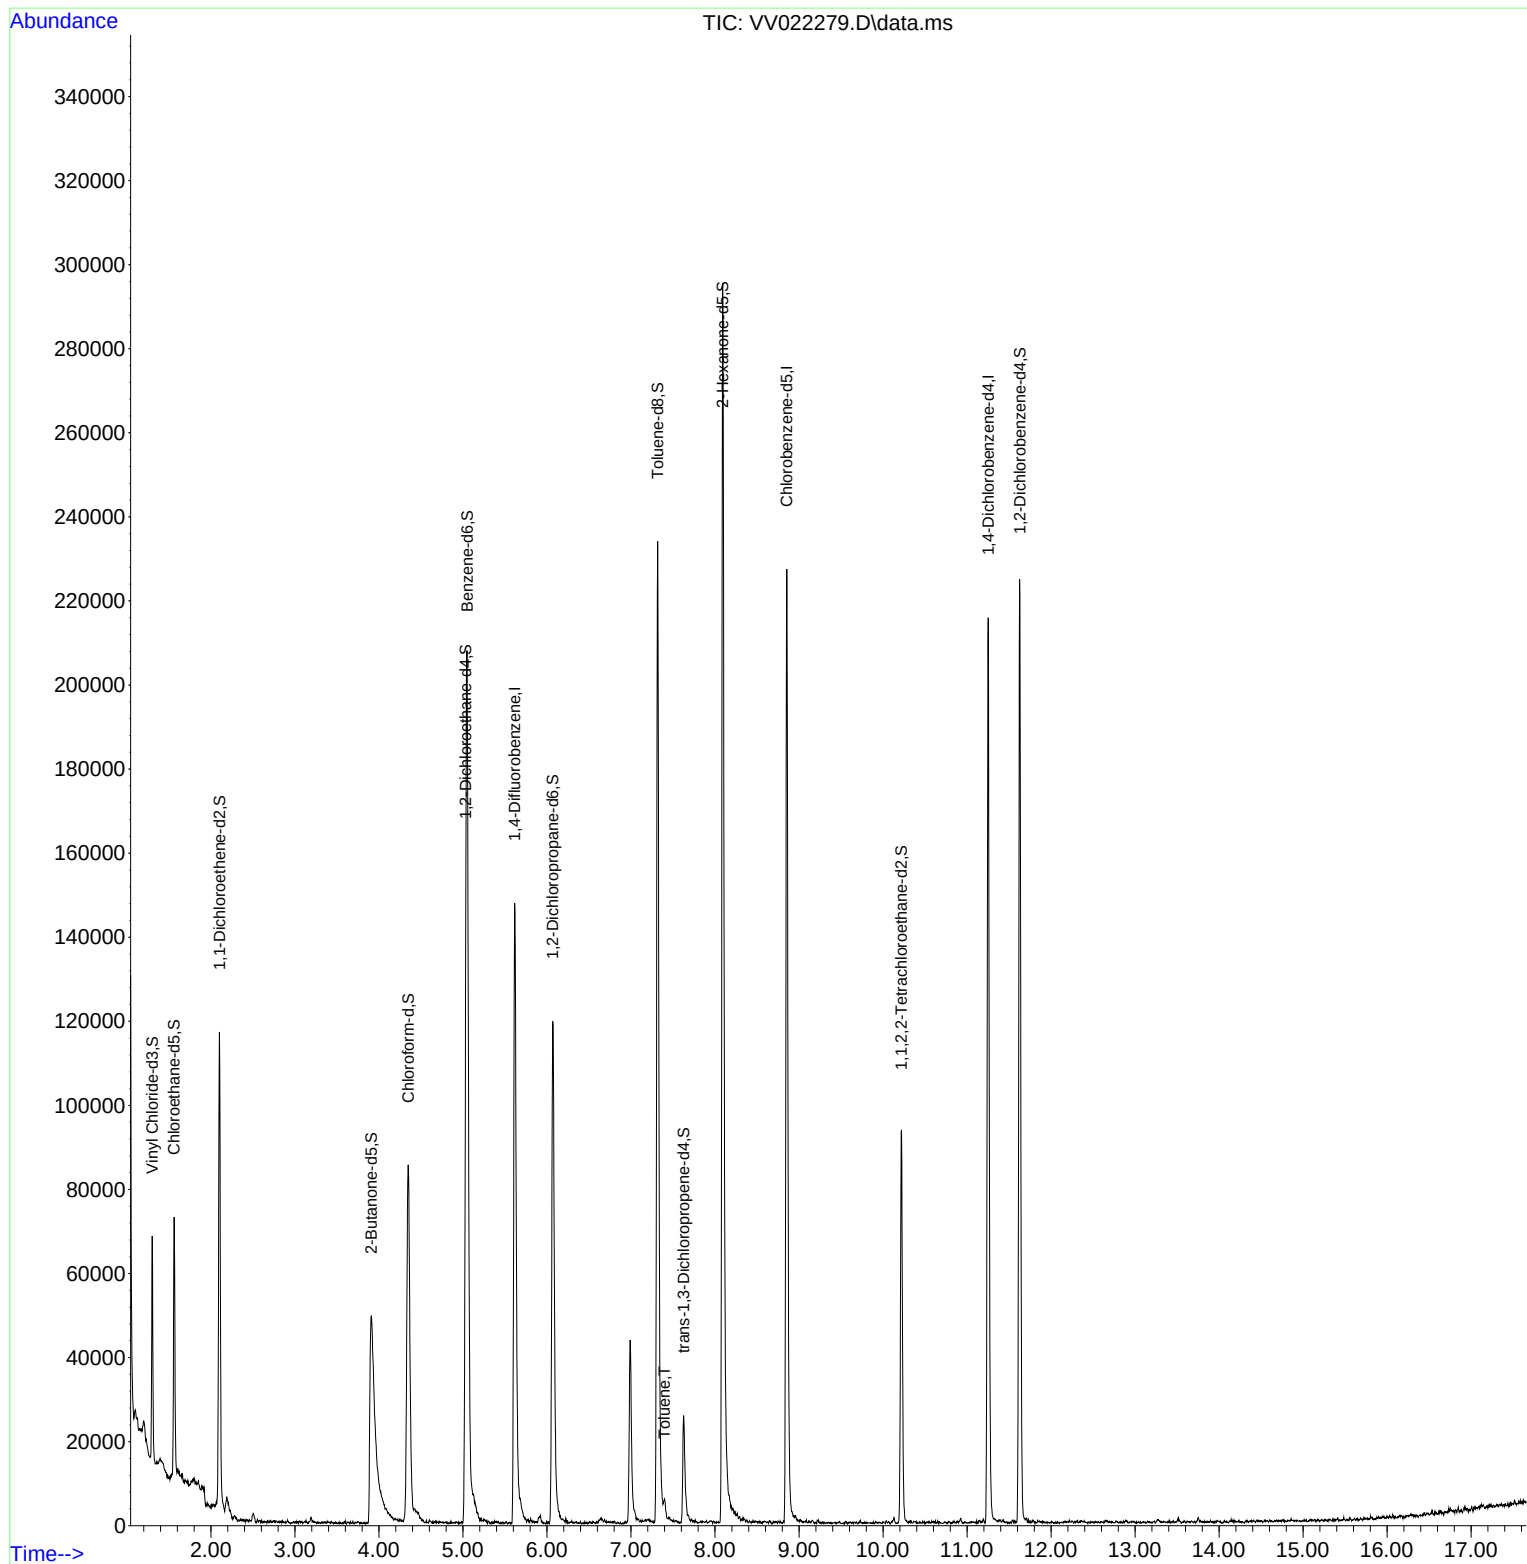

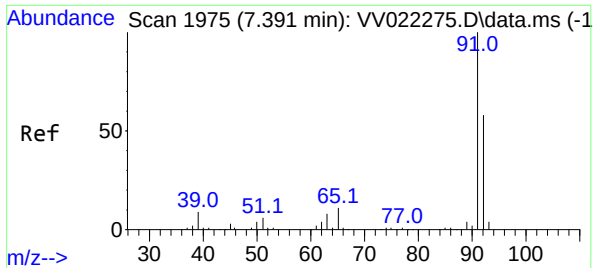

#42
Toluene
Concen: 0.094 ug/L
RT: 7.394 min Scan# 1976
Delta R.T. 0.003 min
Lab File: VV022279.D
Acq: 23 Sep 2021 13:15

Instrument :
MSVOA_V
ClientSampleId :
VBLK209

Tgt Ion: 91 Resp: 3378
Ion Ratio Lower Upper
91 100
92 52.9 40.6 75.4

