

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022281.D
 Acq On : 23 Sep 2021 14:05
 Operator : SY/MD
 Sample : M3814-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6X7

Quant Time: Sep 24 03:44:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 03:31:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	124029	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	122018	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	57589	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	23419	3.747	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.000%
7) Chloroethane-d5	1.561	69	22742	3.110	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	62.200%#
11) 1,1-Dichloroethene-d2	2.105	63	34702	2.329	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	46.600%#
20) 2-Butanone-d5	3.879	46	101349	39.683	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.360%
24) Chloroform-d	4.355	84	61210	3.415	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	68.200%#
26) 1,2-Dichloroethane-d4	5.037	65	30920	3.610	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.200%
32) Benzene-d6	5.053	84	118712	3.460	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	69.200%#
36) 1,2-Dichloropropane-d6	6.075	67	41578	3.880	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	77.600%
41) Toluene-d8	7.320	98	99058	3.197	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	64.000%#
43) trans-1,3-Dichloroprop...	7.628	79	11441	3.496	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	70.000%
46) 2-Hexanone-d5	8.091	63	79258	38.952	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.900%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	35146	3.896	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	78.000%
66) 1,2-Dichlorobenzene-d4	11.628	152	42867	3.966	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	79.400%#
Target Compounds					Qvalue	
13) Acetone	2.162	43	9733	6.722	ug/L	90
42) Toluene	7.400	91	6050	0.178	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022281.D
Acq On : 23 Sep 2021 14:05
Operator : SY/MD
Sample : M3814-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6X7

Quant Time: Sep 24 03:44:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 24 03:31:01 2021
Response via : Initial Calibration




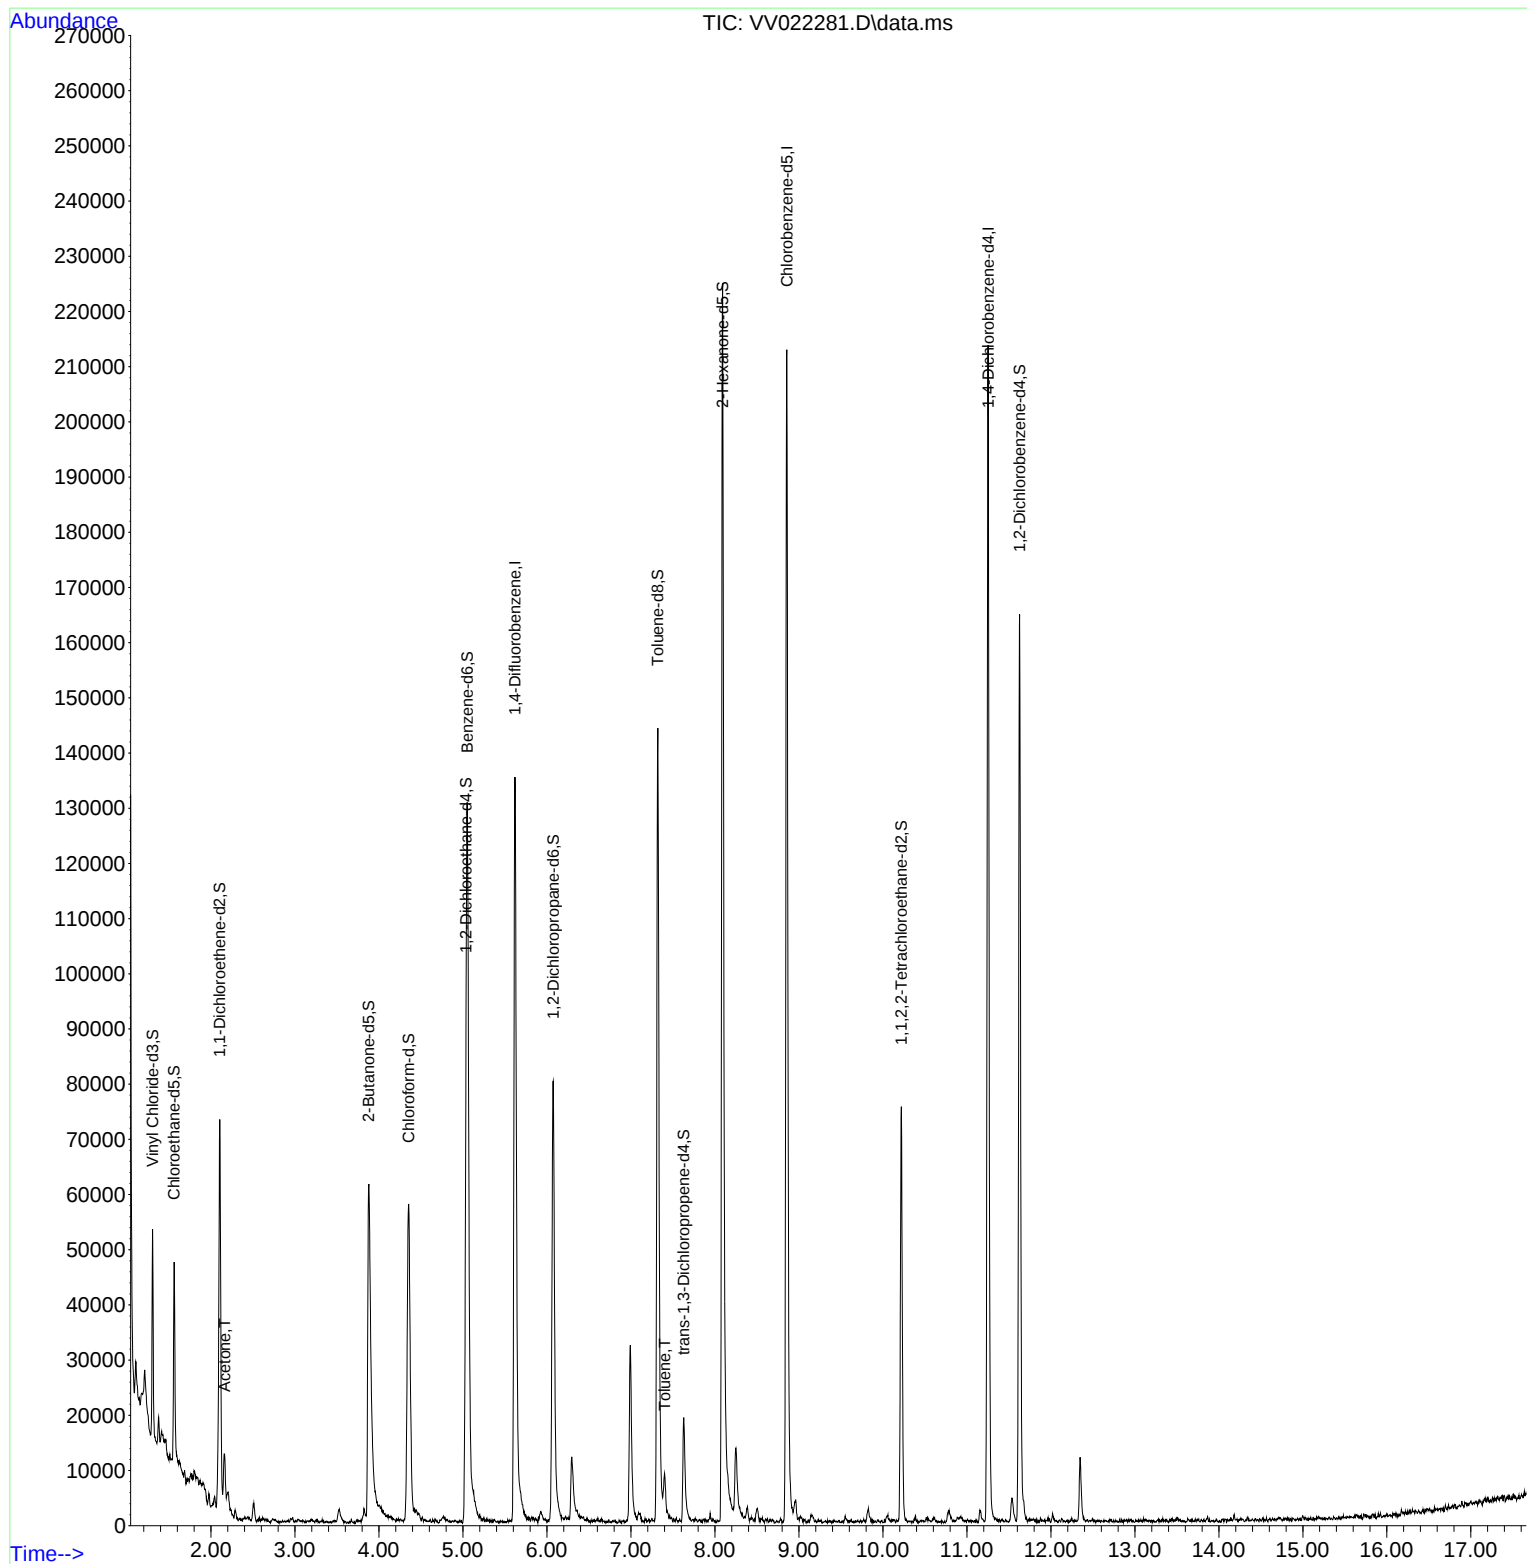


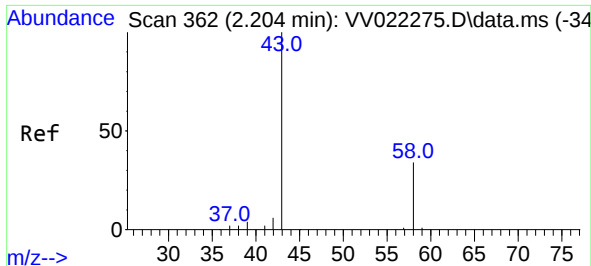

#13
Acetone
Concen: 6.722 ug/L
RT: 2.162 min Scan# 349
Delta R.T. -0.042 min
Lab File: VV022281.D
Acq: 23 Sep 2021 14:05

Instrument :
MSVOA_V
ClientSampleId :
GB6X7

Tgt Ion: 43 Resp: 9733
Ion Ratio Lower Upper
43 100
58 38.7 0.0 66.2

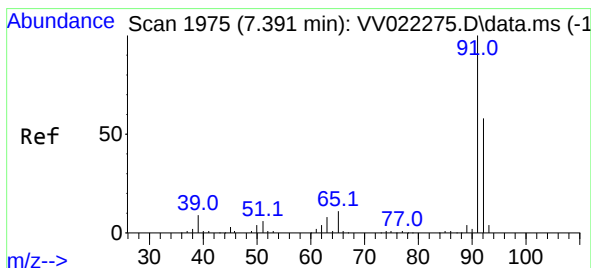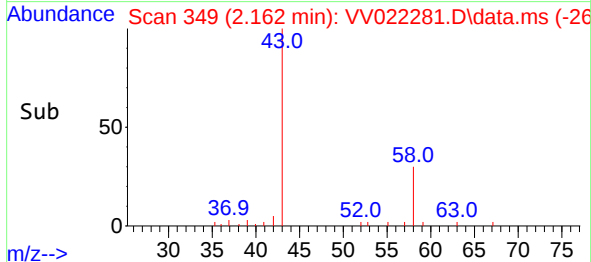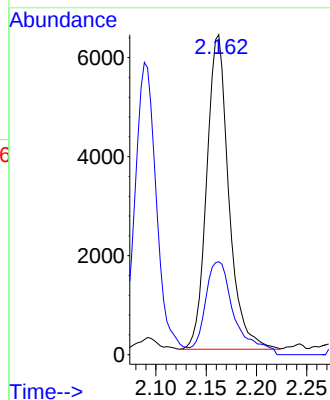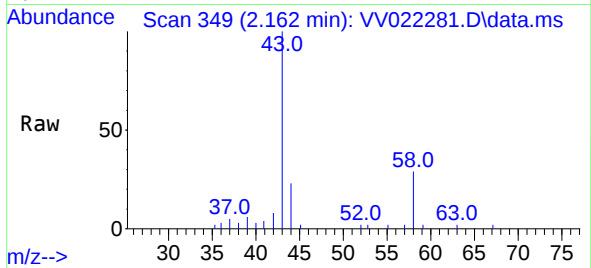

#42
Toluene
Concen: 0.178 ug/L
RT: 7.400 min Scan# 1978
Delta R.T. 0.010 min
Lab File: VV022281.D
Acq: 23 Sep 2021 14:05

Tgt Ion: 91 Resp: 6050
Ion Ratio Lower Upper
91 100
92 57.6 40.6 75.4

