

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW092321\
 Data File : VW022286.D
 Acq On : 23 Sep 2021 16:08
 Operator : SY/MD
 Sample : M3878-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2P3

Quant Time: Sep 24 03:45:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 03:31:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	129717	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	131784	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	58938	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	32011	4.897	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.000%
7) Chloroethane-d5	1.564	69	37912	4.956	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.200%
11) 1,1-Dichloroethene-d2	2.101	63	55758	3.578	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.600%
20) 2-Butanone-d5	3.912	46	136811	51.220	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.440%
24) Chloroform-d	4.352	84	89027	4.749	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%
26) 1,2-Dichloroethane-d4	5.037	65	45677	5.100	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.000%
32) Benzene-d6	5.050	84	182747	4.931	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.600%
36) 1,2-Dichloropropane-d6	6.072	67	58319	5.040	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.800%
41) Toluene-d8	7.317	98	156167	4.667	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.400%
43) trans-1,3-Dichloroprop...	7.628	79	15413	4.361	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.200%
46) 2-Hexanone-d5	8.091	63	113577	51.681	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.360%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	46337	4.756	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	95.200%
66) 1,2-Dichlorobenzene-d4	11.628	152	59469	5.376	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.600%
Target Compounds					Qvalue	
42) Toluene	7.400	91	6614	0.180	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022286.D
Acq On : 23 Sep 2021 16:08
Operator : SY/MD
Sample : M3878-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2P3

Quant Time: Sep 24 03:45:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 24 03:31:01 2021
Response via : Initial Calibration

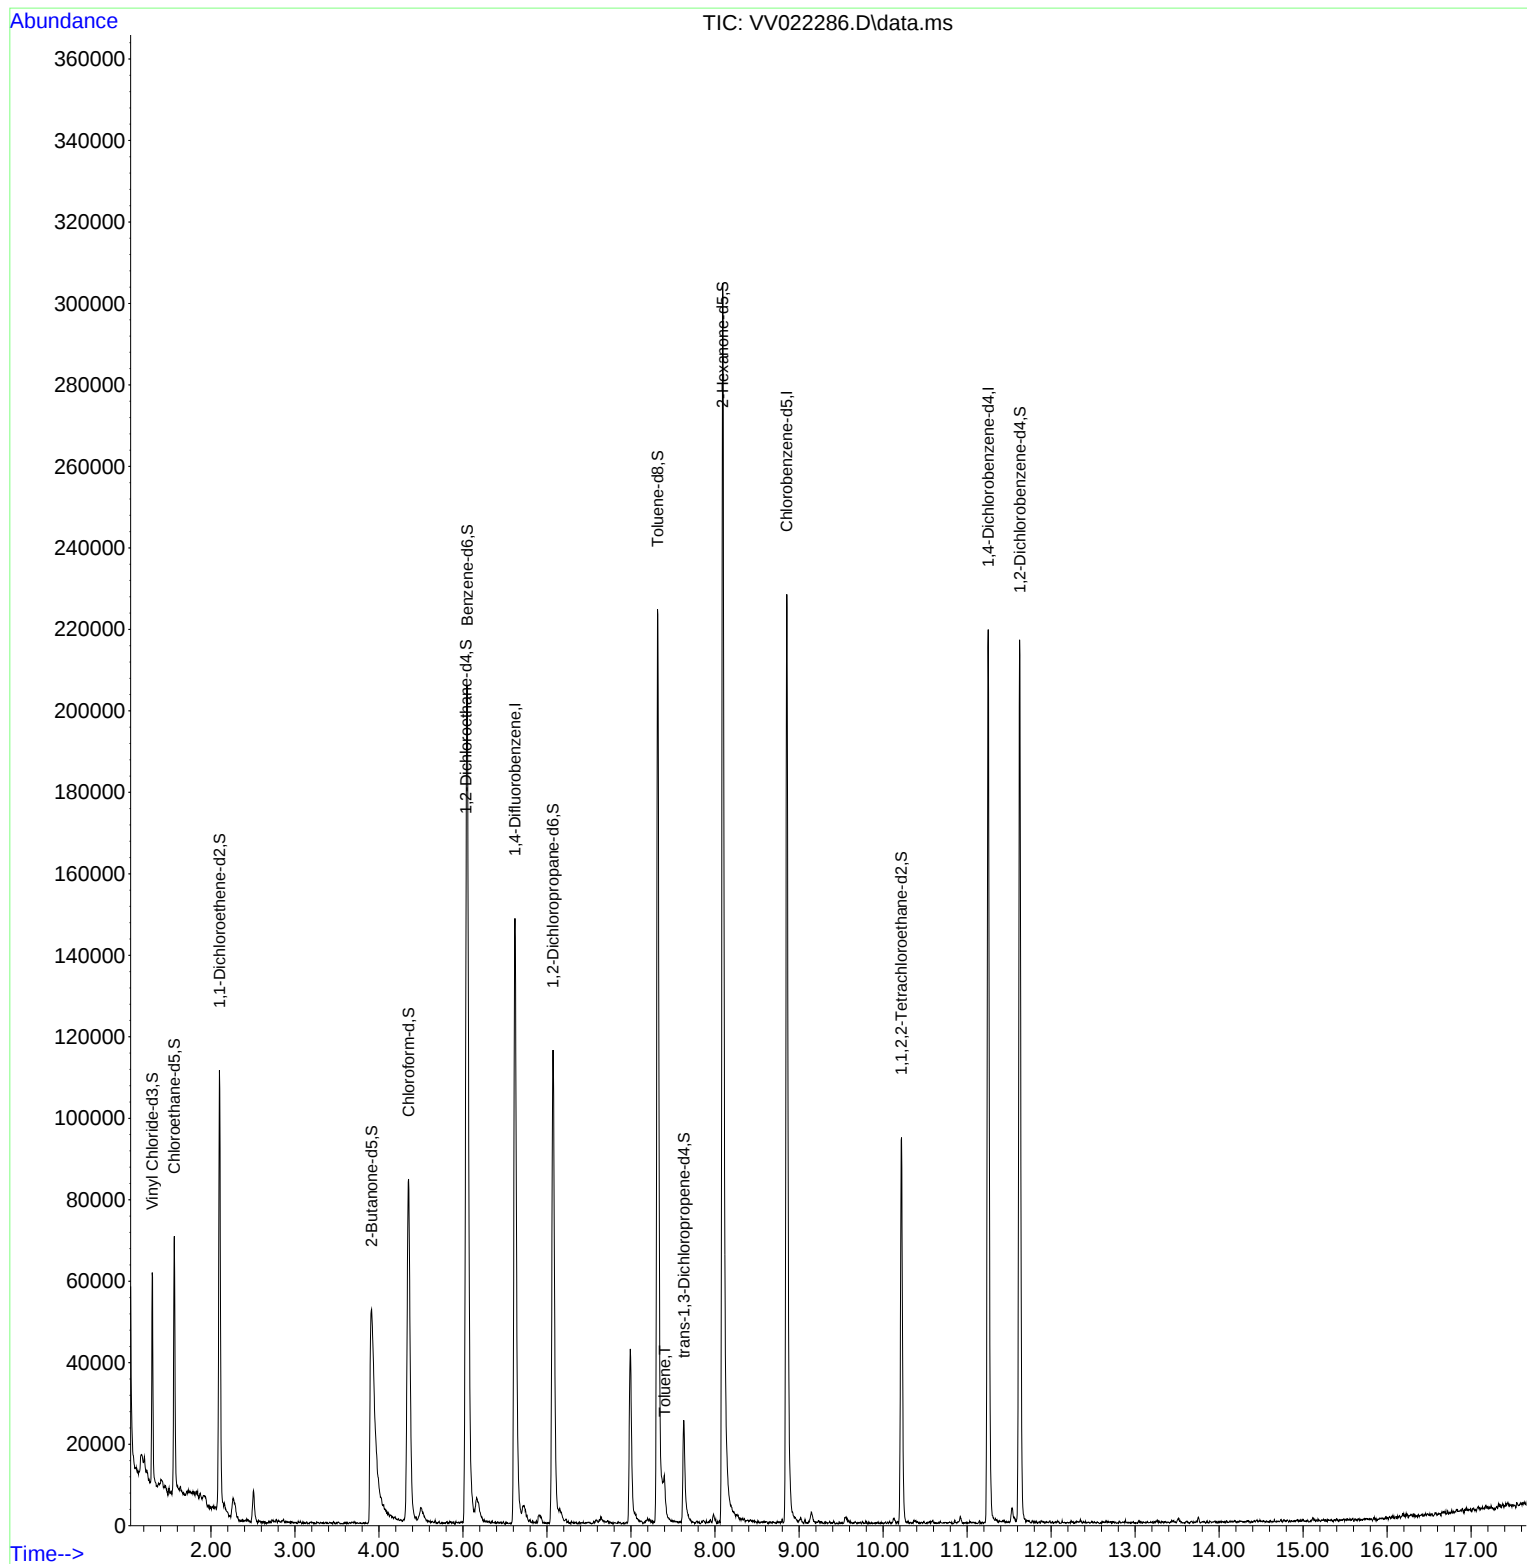

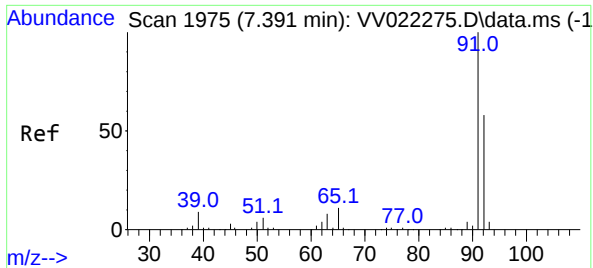

#42
Toluene
Concen: 0.180 ug/L
RT: 7.400 min Scan# 1978
Delta R.T. 0.010 min
Lab File: VV022286.D
Acq: 23 Sep 2021 16:08

Instrument :
MSVOA_V
ClientSampleId :
EW2P3

Tgt Ion: 91 Resp: 6614
Ion Ratio Lower Upper
91 100
92 62.8 40.6 75.4

