

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022289.D
 Acq On : 23 Sep 2021 17:18
 Operator : SY/MD
 Sample : M3814-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6Y0

Quant Time: Sep 24 03:46:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 03:31:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	126322	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	128022	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	56741	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	28754	4.517	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	90.400%	
7) Chloroethane-d5	1.565	69	34863	4.680	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.600%	
11) 1,1-Dichloroethene-d2	2.105	63	48863	3.220	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	64.400%	
20) 2-Butanone-d5	3.886	46	117634	45.224	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	90.440%	
24) Chloroform-d	4.352	84	80508	4.410	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.200%	
26) 1,2-Dichloroethane-d4	5.034	65	40725	4.669	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.400%	
32) Benzene-d6	5.053	84	165979	4.611	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.200%	
36) 1,2-Dichloropropane-d6	6.072	67	54778	4.873	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.400%	
41) Toluene-d8	7.320	98	138327	4.255	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.200%	
43) trans-1,3-Dichloroprop...	7.625	79	14076	4.099	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.000%	
46) 2-Hexanone-d5	8.092	63	99516	46.614	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	93.220%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	41241	4.358	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	87.200%	
66) 1,2-Dichlorobenzene-d4	11.628	152	53939	5.065	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.400%	
Target Compounds					Qvalue	
13) Acetone	2.175	43	27374	18.561	ug/L	95
42) Toluene	7.404	91	2704	0.076	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022289.D
Acq On : 23 Sep 2021 17:18
Operator : SY/MD
Sample : M3814-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6Y0

Quant Time: Sep 24 03:46:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 24 03:31:01 2021
Response via : Initial Calibration




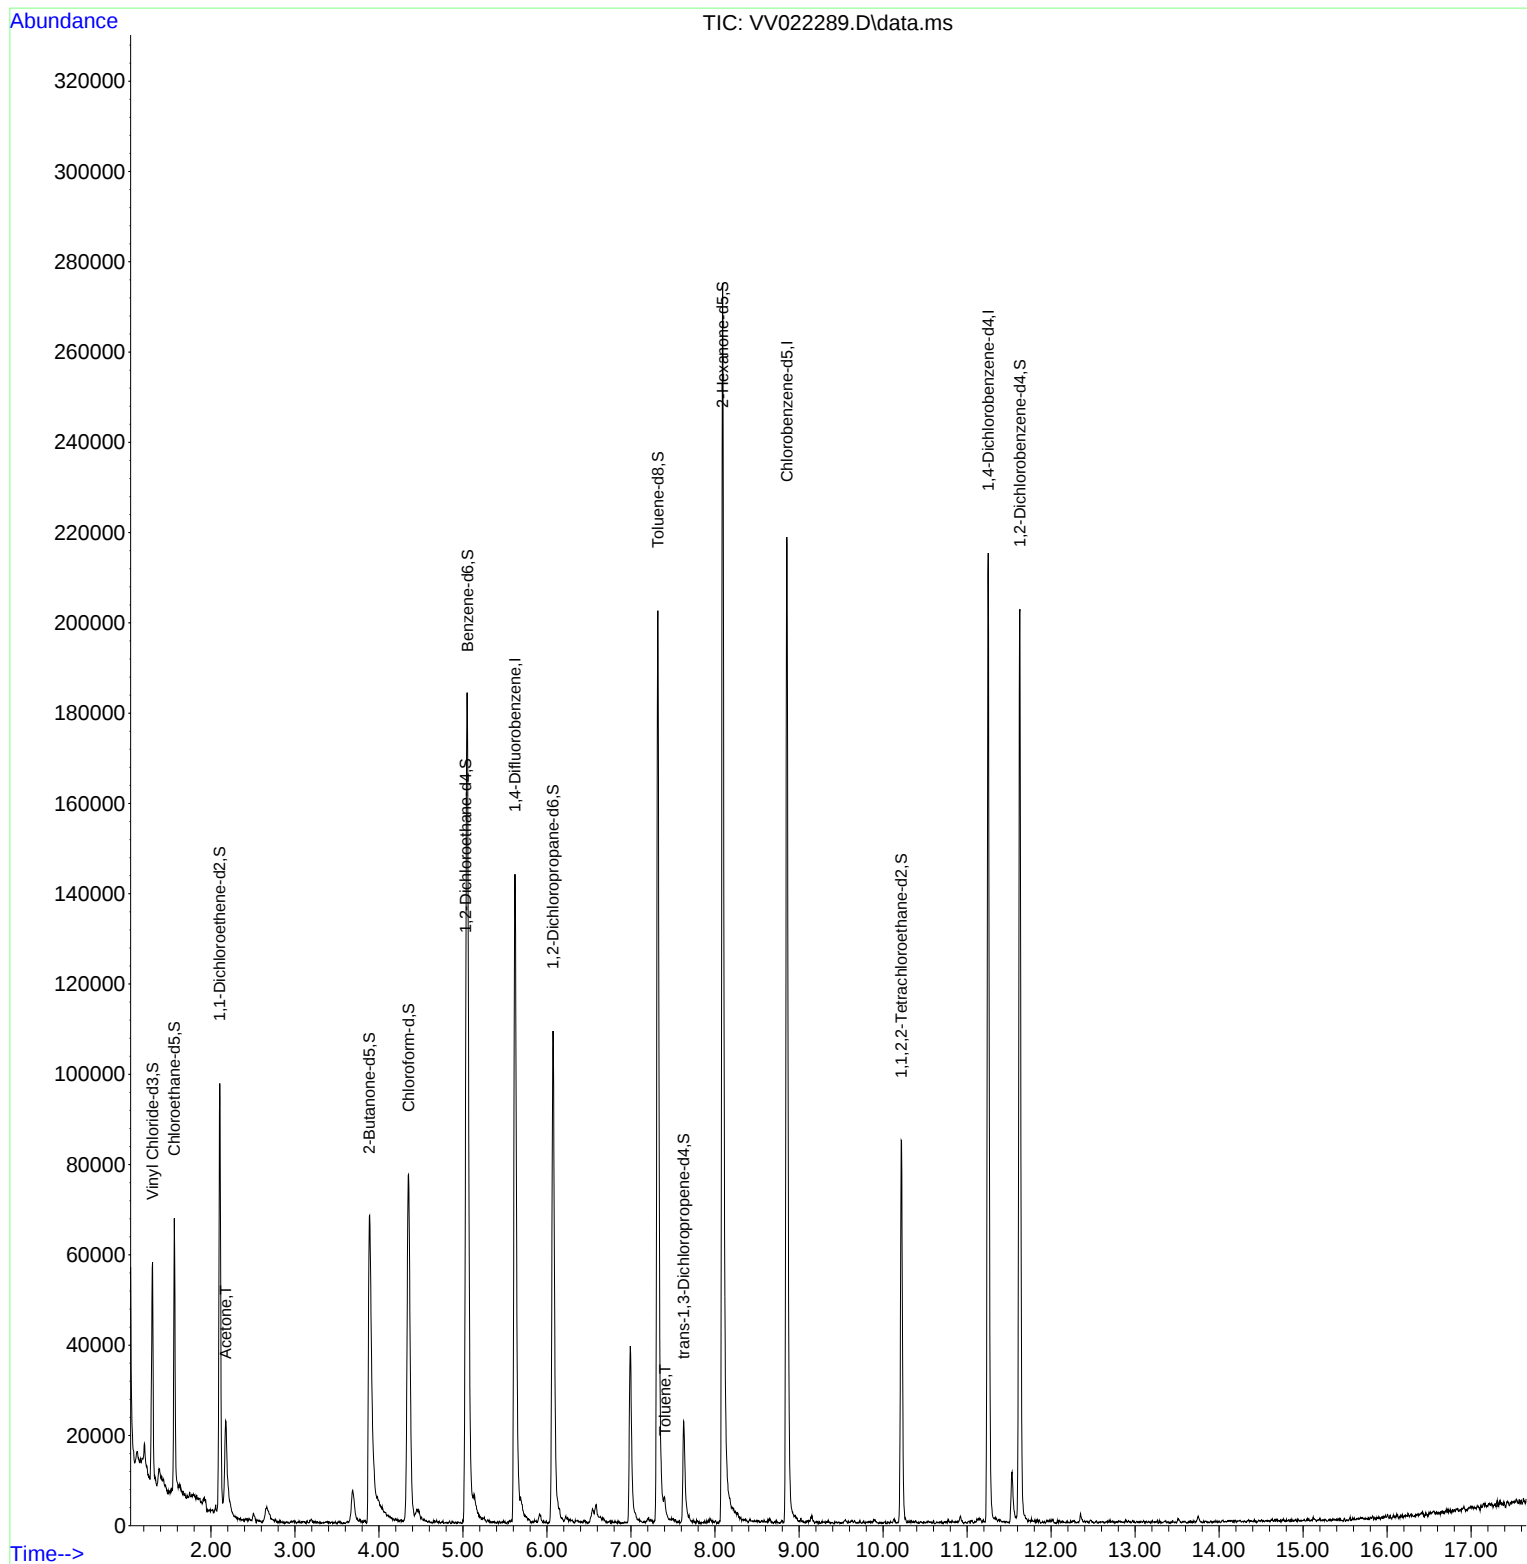


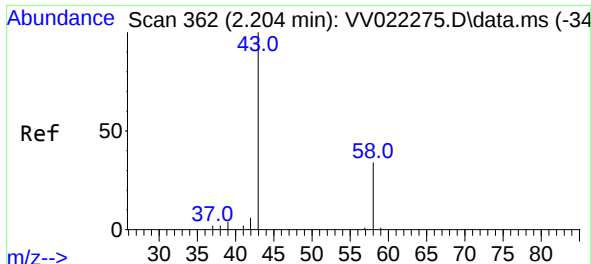

#13
Acetone
Concen: 18.561 ug/L
RT: 2.175 min Scan# 353
Delta R.T. -0.029 min
Lab File: VV022289.D
Acq: 23 Sep 2021 17:18

Instrument :
MSVOA_V
ClientSampleId :
GB6Y0

Tgt Ion: 43 Resp: 27374
Ion Ratio Lower Upper
43 100
58 30.0 0.0 66.2

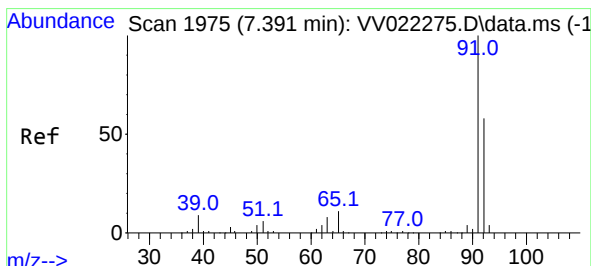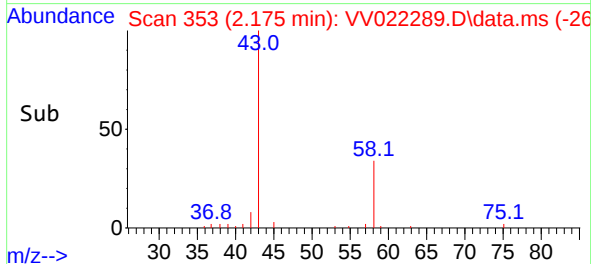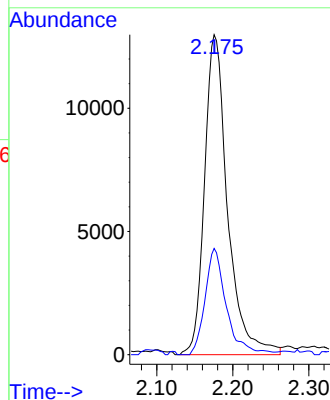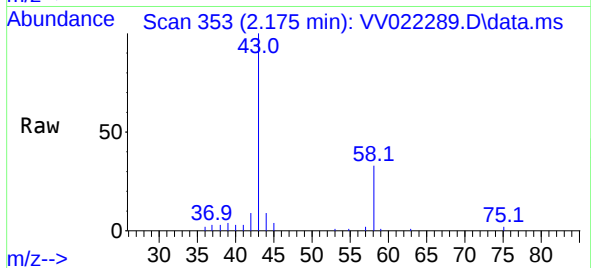

#42
Toluene
Concen: 0.076 ug/L
RT: 7.404 min Scan# 1979
Delta R.T. 0.013 min
Lab File: VV022289.D
Acq: 23 Sep 2021 17:18

Tgt Ion: 91 Resp: 2704
Ion Ratio Lower Upper
91 100
92 55.0 40.6 75.4

