

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022290.D
 Acq On : 23 Sep 2021 17:43
 Operator : SY/MD
 Sample : M3814-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Sep 24 03:46:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 03:31:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	116252	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	120771	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	53093	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	28216	4.817	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	96.400%	
7) Chloroethane-d5	1.561	69	35511	5.180	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	103.600%	
11) 1,1-Dichloroethene-d2	2.101	63	50088	3.586	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	71.800%	
20) 2-Butanone-d5	3.912	46	123104	51.426	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	102.860%	
24) Chloroform-d	4.349	84	82565	4.914	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.200%	
26) 1,2-Dichloroethane-d4	5.037	65	40897	5.095	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.800%	
32) Benzene-d6	5.050	84	164884	4.855	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.200%	
36) 1,2-Dichloropropane-d6	6.072	67	53306	5.026	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.600%	
41) Toluene-d8	7.320	98	131204	4.278	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.600%	
43) trans-1,3-Dichloroprop...	7.628	79	13360	4.125	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	82.400%	
46) 2-Hexanone-d5	8.095	63	104538	51.906	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	103.820%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	42494	4.760	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.200%	
66) 1,2-Dichlorobenzene-d4	11.628	152	52841	5.303	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	106.000%	
Target Compounds					Qvalue	
42) Toluene	7.400	91	2857	0.085	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022290.D
Acq On : 23 Sep 2021 17:43
Operator : SY/MD
Sample : M3814-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Sep 24 03:46:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 24 03:31:01 2021
Response via : Initial Calibration

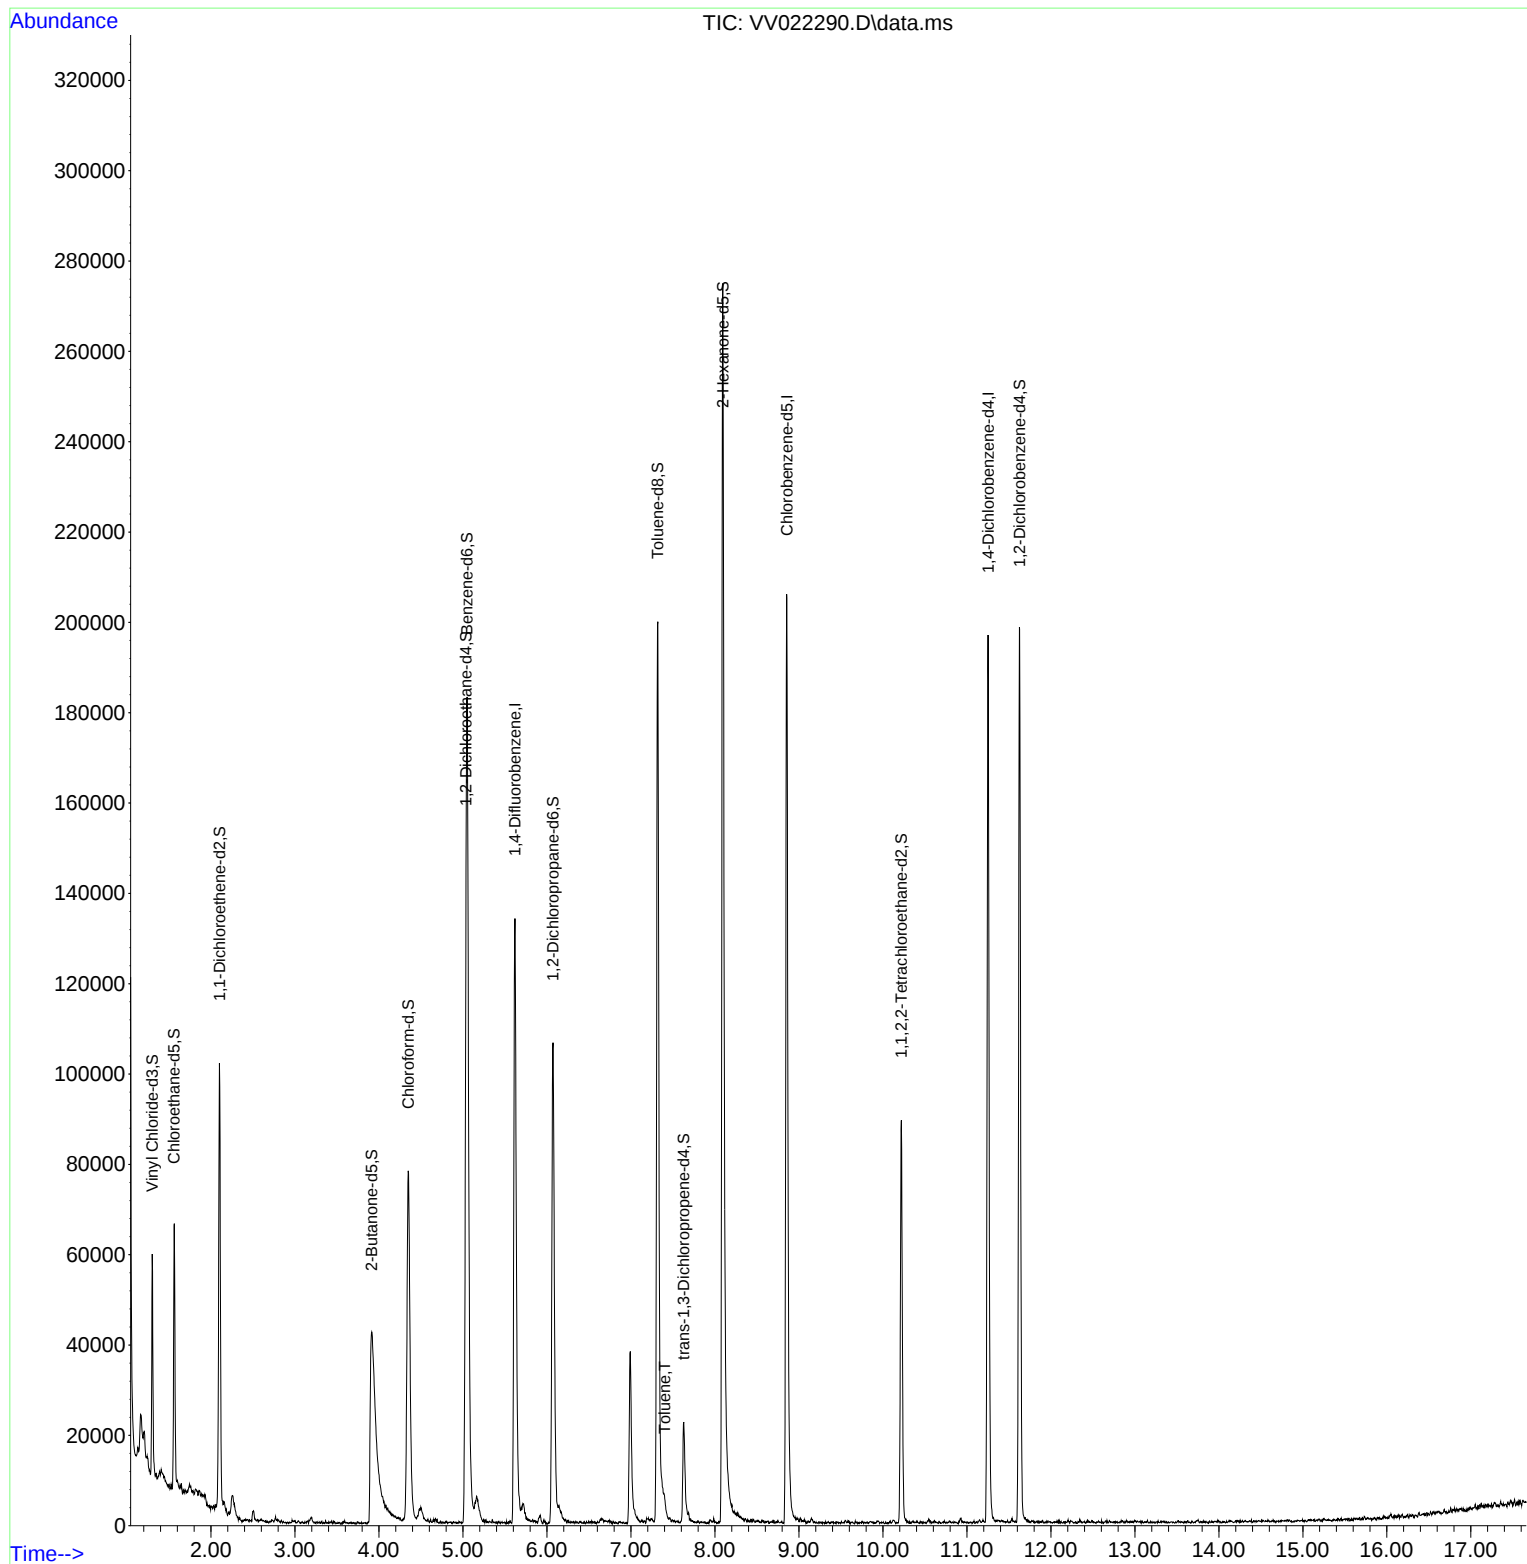

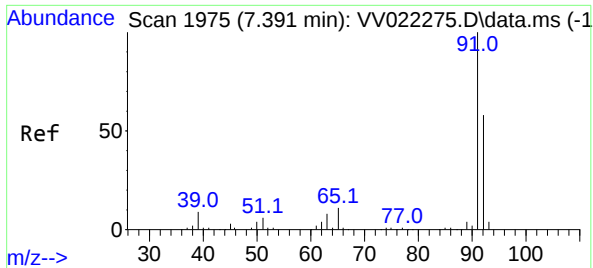

#42
Toluene
Concen: 0.085 ug/L
RT: 7.400 min Scan# 1978
Delta R.T. 0.010 min
Lab File: VV022290.D
Acq: 23 Sep 2021 17:43

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 91 Resp: 2857
Ion Ratio Lower Upper
91 100
92 58.6 40.6 75.4

