

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW092321\
 Data File : VW022308.D
 Acq On : 24 Sep 2021 01:27
 Operator : SY/MD
 Sample : M3878-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2P5

Quant Time: Sep 24 05:11:57 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 05:07:58 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	117860	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	118601	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	52030	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	29859	5.028	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	100.600%	
7) Chloroethane-d5	1.561	69	36985	5.322	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	106.400%	
11) 1,1-Dichloroethene-d2	2.105	63	51593	3.644	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.800%	
20) 2-Butanone-d5	3.883	46	130796	53.894	ug/L	-0.04
Spiked Amount	50.000	Range 40 - 130	Recovery	=	107.780%	
24) Chloroform-d	4.349	84	86689	5.089	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.800%	
26) 1,2-Dichloroethane-d4	5.037	65	43074	5.293	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.800%	
32) Benzene-d6	5.050	84	173230	5.194	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.800%	
36) 1,2-Dichloropropane-d6	6.072	67	58069	5.576	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	111.600%	
41) Toluene-d8	7.320	98	145754	4.840	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.800%	
43) trans-1,3-Dichloroprop...	7.625	79	13766	4.328	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	86.600%	
46) 2-Hexanone-d5	8.088	63	101946	51.545	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	103.100%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	41980	4.788	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.800%	
66) 1,2-Dichlorobenzene-d4	11.628	152	54862	5.618	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	112.400%	
Target Compounds					Qvalue	
13) Acetone	2.169	43	13104	9.523	ug/L	97
42) Toluene	7.400	91	4158	0.126	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022308.D
Acq On : 24 Sep 2021 01:27
Operator : SY/MD
Sample : M3878-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2P5

Quant Time: Sep 24 05:11:57 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 24 05:07:58 2021
Response via : Initial Calibration




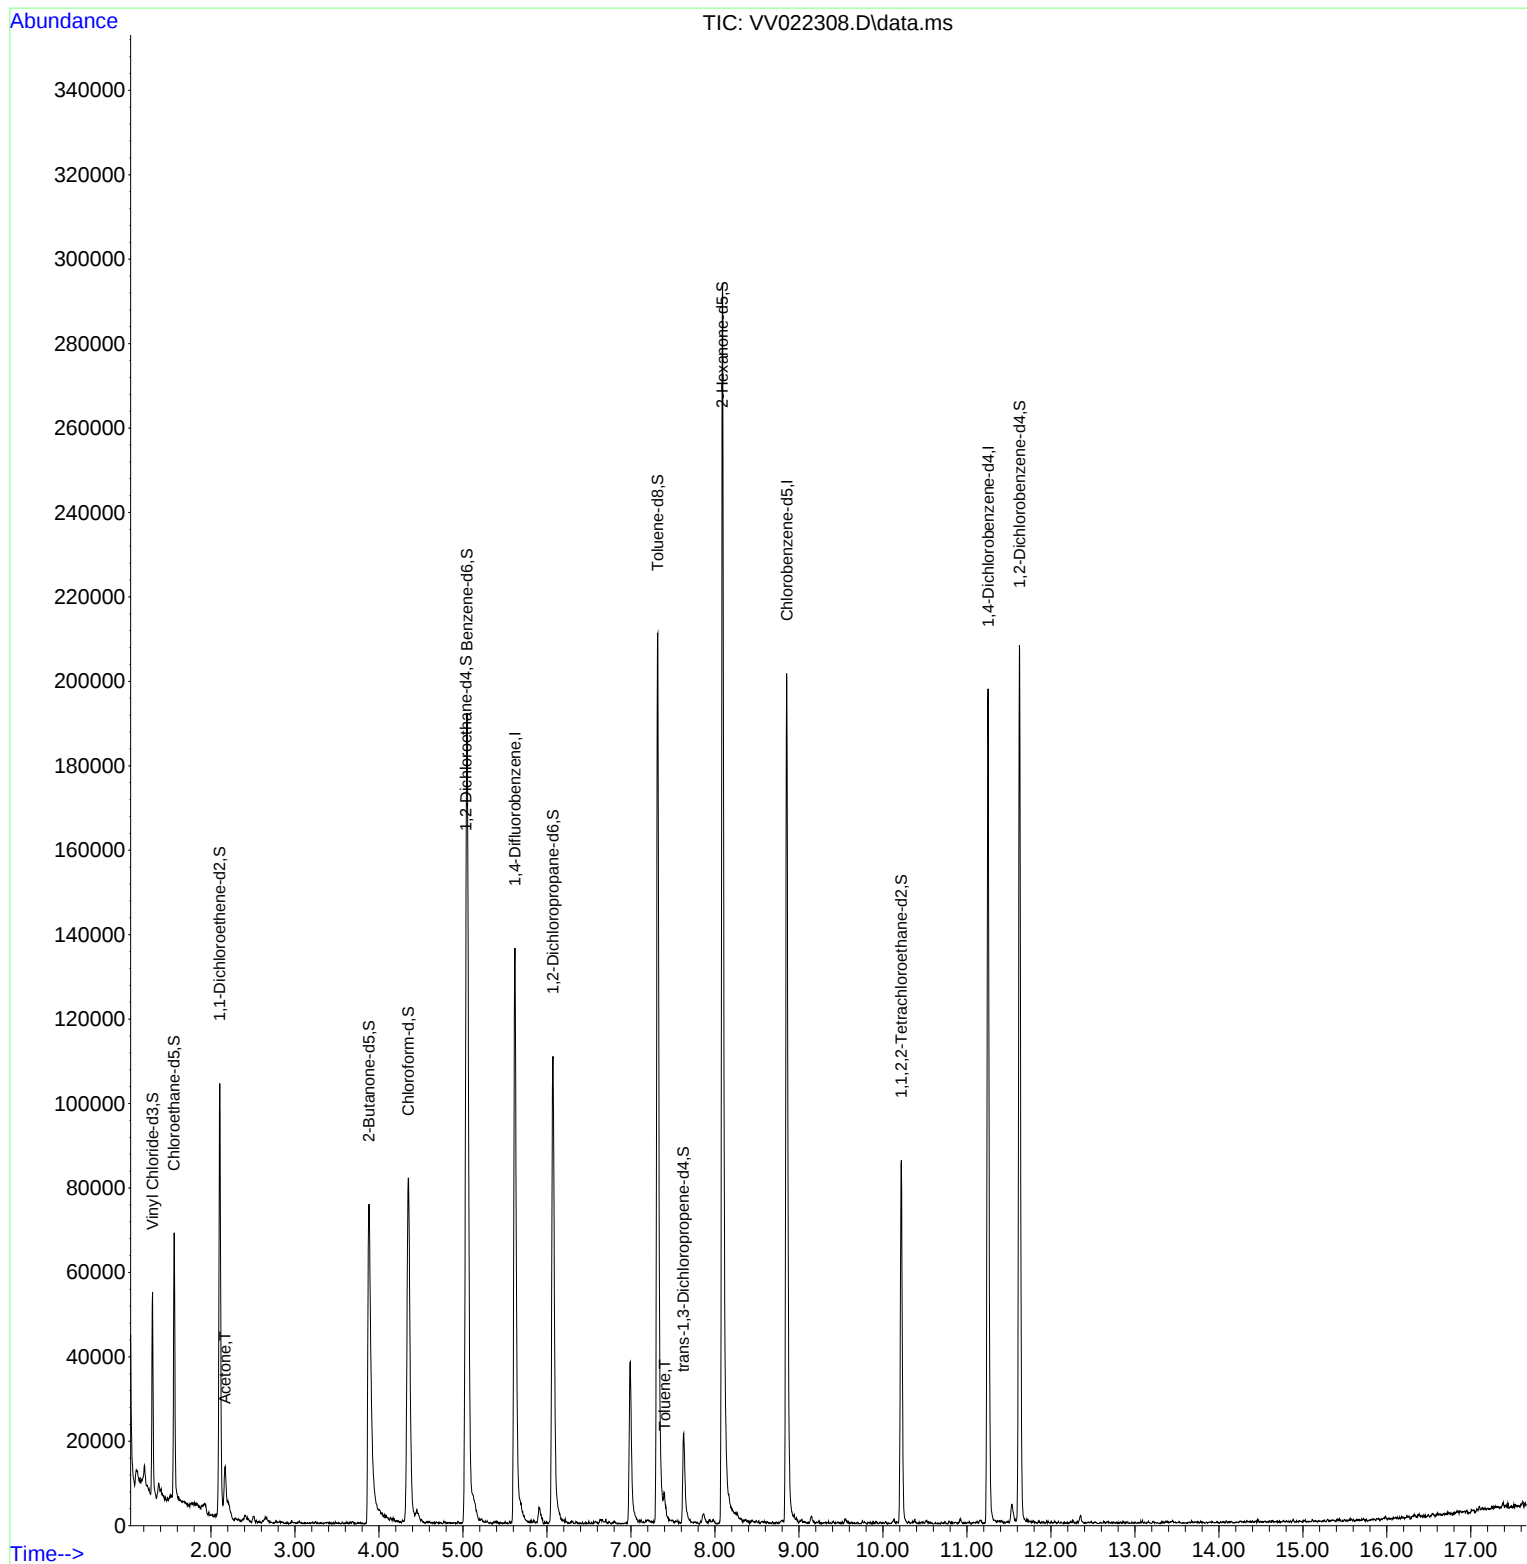


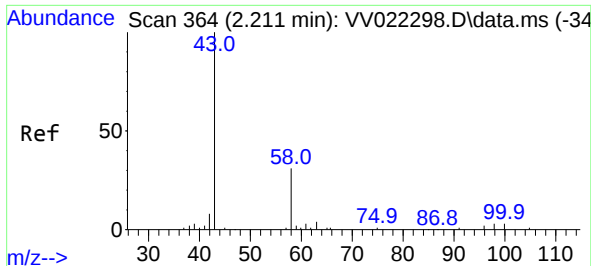

#13
Acetone
Concen: 9.523 ug/L
RT: 2.169 min Scan# 351
Delta R.T. -0.042 min
Lab File: VV022308.D
Acq: 24 Sep 2021 01:27

Instrument :
MSVOA_V
ClientSampleId :
EW2P5

Tgt Ion: 43 Resp: 13104
Ion Ratio Lower Upper
43 100
58 31.5 0.0 66.2

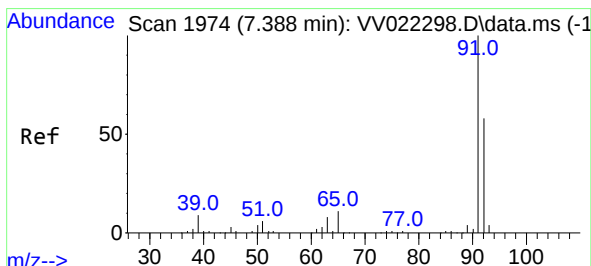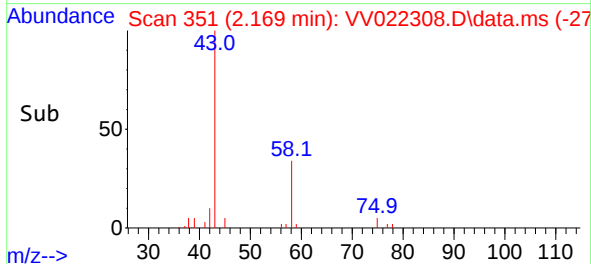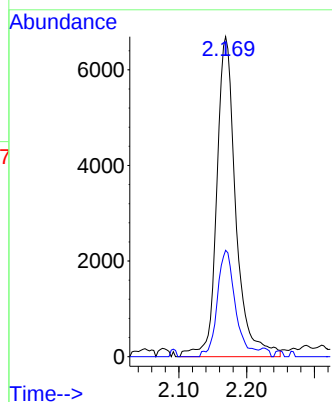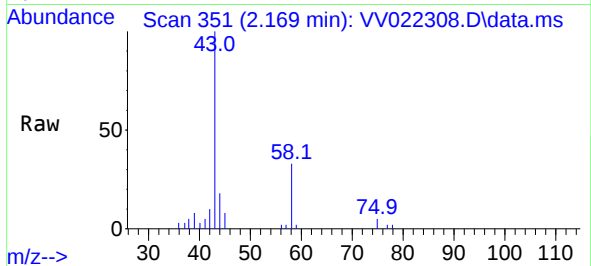

#42
Toluene
Concen: 0.126 ug/L
RT: 7.400 min Scan# 1978
Delta R.T. 0.013 min
Lab File: VV022308.D
Acq: 24 Sep 2021 01:27

Tgt Ion: 91 Resp: 4158
Ion Ratio Lower Upper
91 100
92 60.6 40.6 75.4

