

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW092321\
 Data File : VW022309.D
 Acq On : 24 Sep 2021 01:52
 Operator : SY/MD
 Sample : M3878-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2P6

Quant Time: Sep 24 05:12:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 24 05:07:58 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	117288	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	116226	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	50539	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	29577	5.004	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 100.000%		
7) Chloroethane-d5	1.561	69	36996	5.349	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 107.000%		
11) 1,1-Dichloroethene-d2	2.105	63	52364	3.716	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 74.400%		
20) 2-Butanone-d5	3.880	46	125206	51.842	ug/L	-0.04
Spiked Amount	50.000	Range 40 - 130	Recovery	= 103.680%		
24) Chloroform-d	4.352	84	89166	5.260	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 105.200%		
26) 1,2-Dichloroethane-d4	5.034	65	43926	5.424	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 108.400%		
32) Benzene-d6	5.050	84	176688	5.406	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 108.200%		
36) 1,2-Dichloropropane-d6	6.072	67	58004	5.683	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 113.600%		
41) Toluene-d8	7.317	98	142630	4.833	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 96.600%		
43) trans-1,3-Dichloroprop...	7.629	79	13203	4.235	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 84.800%		
46) 2-Hexanone-d5	8.088	63	101589	52.414	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 104.820%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42185	4.910	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 98.200%		
66) 1,2-Dichlorobenzene-d4	11.628	152	54287	5.723	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 114.400%		
Target Compounds						Qvalue
13) Acetone	2.166	43	2063	1.507	ug/L	71
42) Toluene	7.400	91	5102	0.158	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022309.D
Acq On : 24 Sep 2021 01:52
Operator : SY/MD
Sample : M3878-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2P6

Quant Time: Sep 24 05:12:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 24 05:07:58 2021
Response via : Initial Calibration




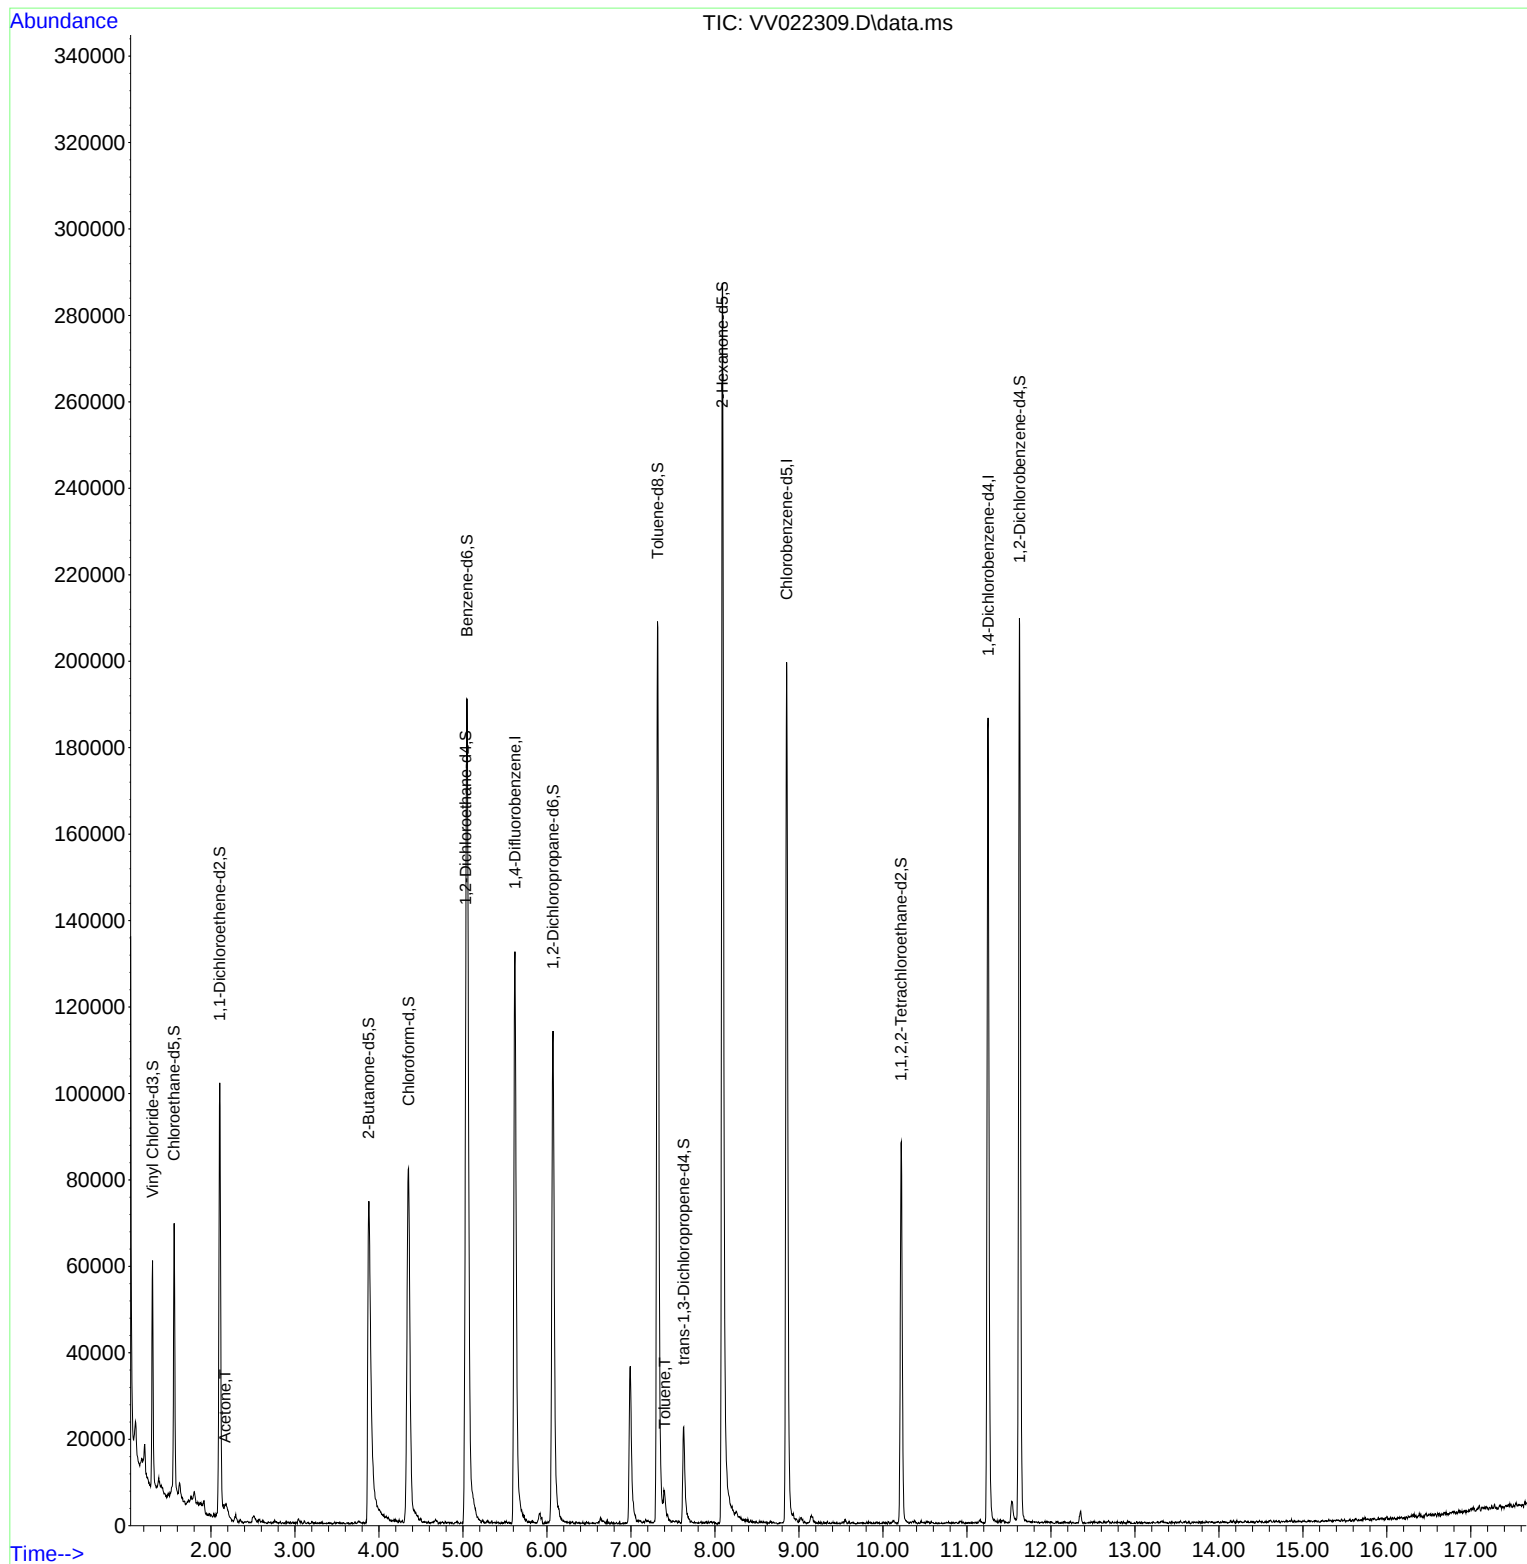


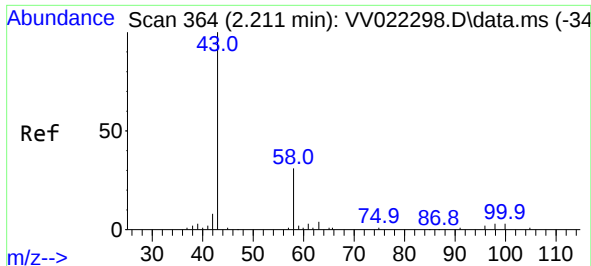

#13
Acetone
Concen: 1.507 ug/L
RT: 2.166 min Scan# 350
Delta R.T. -0.045 min
Lab File: VV022309.D
Acq: 24 Sep 2021 01:52

Instrument :
MSVOA_V
ClientSampleId :
EW2P6

Tgt Ion: 43 Resp: 2063
Ion Ratio Lower Upper
43 100
58 16.8 0.0 66.2

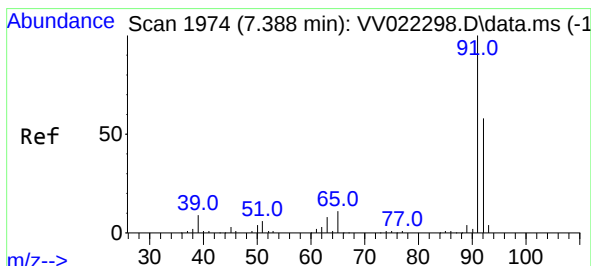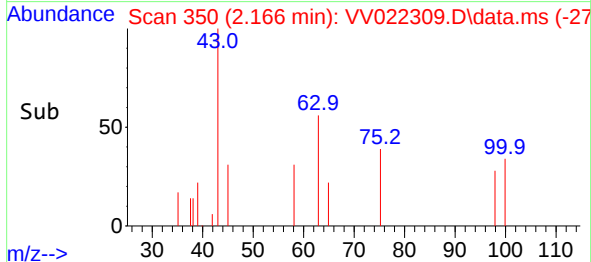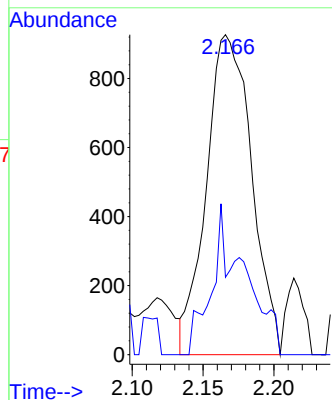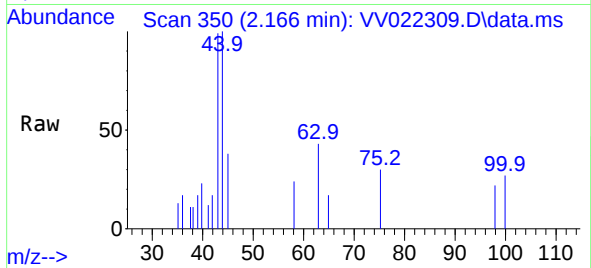

#42
Toluene
Concen: 0.158 ug/L
RT: 7.400 min Scan# 1978
Delta R.T. 0.013 min
Lab File: VV022309.D
Acq: 24 Sep 2021 01:52

Tgt Ion: 91 Resp: 5102
Ion Ratio Lower Upper
91 100
92 57.8 40.6 75.4

