

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022283.D
 Acq On : 23 Sep 2021 14:54
 Operator : SY/MD
 Sample : M3814-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6X9

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022283.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	43098	48874	10.98%	1.416%
2	1.378	100	105	110	rBV	4373	5326	1.20%	0.154%
3	1.565	156	163	174	rVB	43400	48970	11.01%	1.419%
4	2.105	322	331	342	rBV	73822	107992	24.27%	3.129%
5	2.166	342	350	364	rVB	20798	33864	7.61%	0.981%
6	2.507	447	456	463	rBV6	2736	4505	1.01%	0.131%
7	2.642	487	498	515	rBV2	3940	10264	2.31%	0.297%
8	3.690	810	824	839	rBV3	6117	16233	3.65%	0.470%
9	3.880	874	883	907	rBV	65505	178717	40.17%	5.179%
10	4.352	1014	1030	1052	rBV3	62483	157599	35.42%	4.567%
11	5.050	1231	1247	1269	rBV3	143218	362985	81.58%	10.518%
12	5.619	1412	1424	1446	rBV	138593	288887	64.93%	8.371%
13	6.072	1552	1565	1585	rBV	87354	184343	41.43%	5.342%
14	6.545	1699	1712	1716	rBV9	2527	5285	1.19%	0.153%
15	6.580	1717	1723	1732	rVB3	3059	5712	1.28%	0.166%
16	6.992	1840	1851	1867	rBV	34041	65811	14.79%	1.907%
17	7.320	1941	1953	1969	rBV	156550	284972	64.05%	8.258%
18	7.629	2039	2049	2064	rBV2	19668	38404	8.63%	1.113%
19	7.944	2139	2147	2156	rBV3	4060	6219	1.40%	0.180%
20	8.092	2181	2193	2214	rBV	246663	444954	100.00%	12.893%
21	8.857	2419	2431	2457	rBV	211670	368148	82.74%	10.668%
22	9.149	2512	2522	2532	rBV8	3177	6264	1.41%	0.182%
23	10.220	2843	2855	2873	rBV	78119	126654	28.46%	3.670%
24	10.387	2898	2907	2917	rVB4	6653	11052	2.48%	0.320%
25	11.252	3165	3176	3194	rBV	213111	334040	75.07%	9.679%
26	11.532	3254	3263	3272	rBV4	8600	15606	3.51%	0.452%
27	11.625	3281	3292	3309	rBV	169637	274835	61.77%	7.964%
28	12.259	3479	3489	3500	rVB2	3027	5228	1.17%	0.151%
29	12.349	3508	3517	3527	rBV5	6034	9262	2.08%	0.268%




Sum of corrected areas: 3451005

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022283.D
Acq On : 23 Sep 2021 14:54
Operator : SY/MD
Sample : M3814-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
GB6X9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

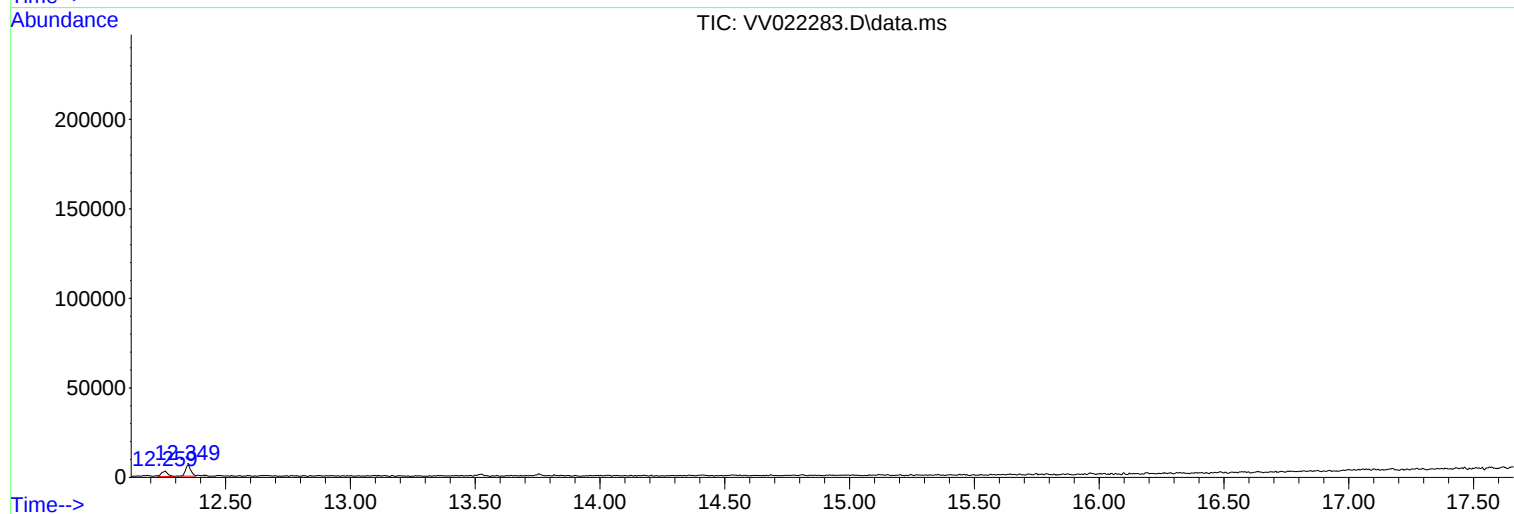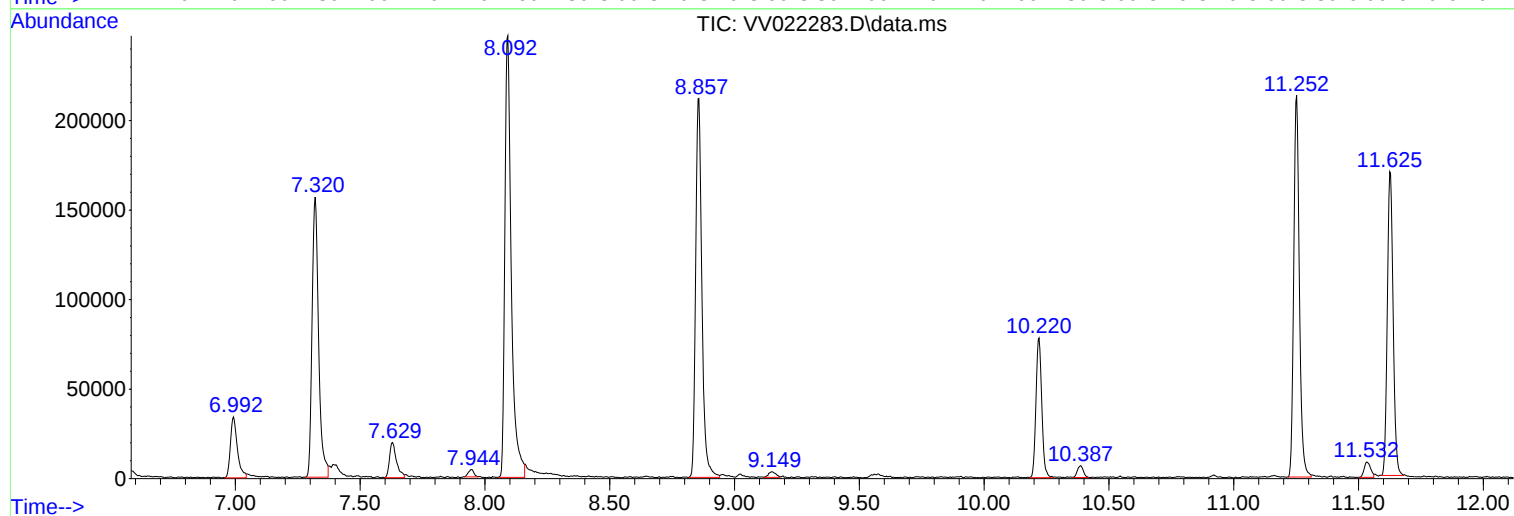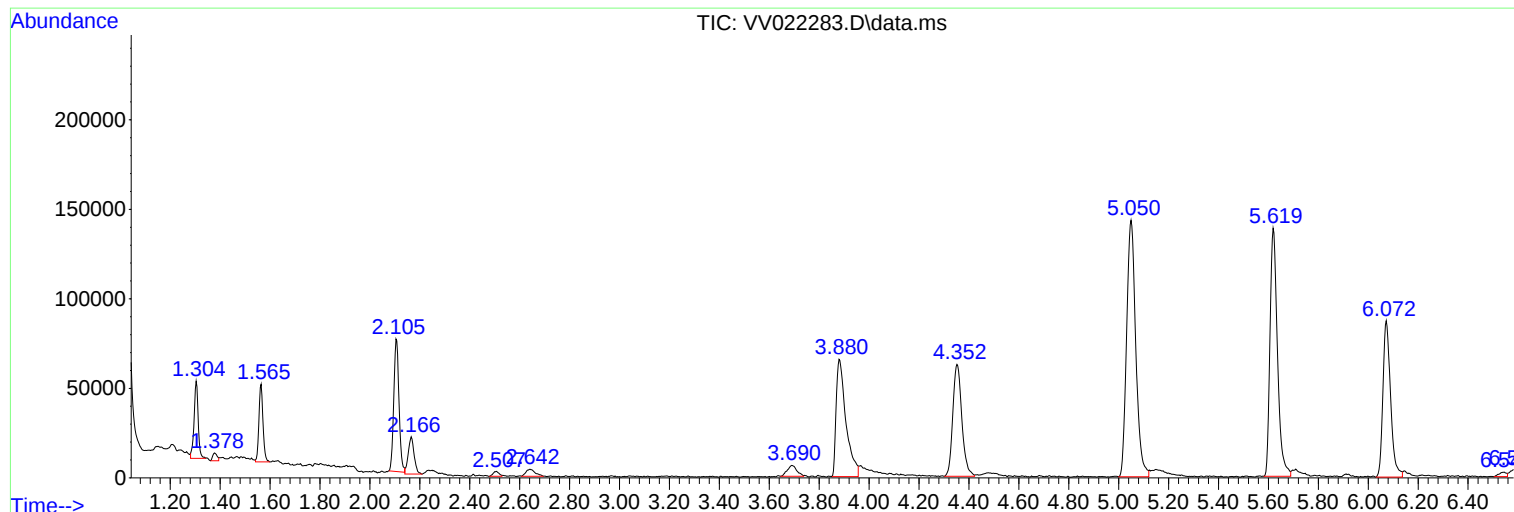

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022283.D
Acq On : 23 Sep 2021 14:54
Operator : SY/MD
Sample : M3814-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6X9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022283.D
Acq On : 23 Sep 2021 14:54
Operator : SY/MD
Sample : M3814-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6X9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
