

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022285.D
 Acq On : 23 Sep 2021 15:43
 Operator : SY/MD
 Sample : M3878-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2J7

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022285.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rVB	49871	52045	9.12%	1.252%
2	1.564	155	163	179	rBV	62209	73260	12.83%	1.763%
3	2.101	321	330	344	rBV	109080	156277	27.38%	3.760%
4	2.506	449	456	470	rVB5	4521	8103	1.42%	0.195%
5	3.908	882	892	926	rBV2	51342	220009	38.54%	5.293%
6	4.352	1010	1030	1052	rBV	84258	213989	37.49%	5.148%
7	5.050	1229	1247	1267	rBV2	204097	504126	88.32%	12.129%
8	5.230	1290	1303	1318	rVB4	6907	16875	2.96%	0.406%
9	5.619	1412	1424	1444	rBV	151337	309461	54.22%	7.445%
10	6.072	1551	1565	1595	rBV2	116833	250425	43.87%	6.025%
11	6.989	1841	1850	1871	rBV	42048	83466	14.62%	2.008%
12	7.320	1939	1953	1972	rBV	220603	403416	70.68%	9.706%
13	7.394	1972	1976	1994	rVB6	6319	12293	2.15%	0.296%
14	7.628	2037	2049	2064	rBV	25771	47353	8.30%	1.139%
15	7.863	2114	2122	2135	rVB7	2776	5763	1.01%	0.139%
16	8.095	2182	2194	2221	rBV	304388	570803	100.00%	13.733%
17	8.853	2419	2430	2459	rBV	226032	383816	67.24%	9.234%
18	10.220	2842	2855	2870	rBV	94178	151455	26.53%	3.644%
19	11.252	3163	3176	3190	rBV	220181	345475	60.52%	8.312%
20	11.625	3278	3292	3313	rBV	215392	347993	60.97%	8.372%




Sum of corrected areas: 4156403

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022285.D
Acq On : 23 Sep 2021 15:43
Operator : SY/MD
Sample : M3878-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

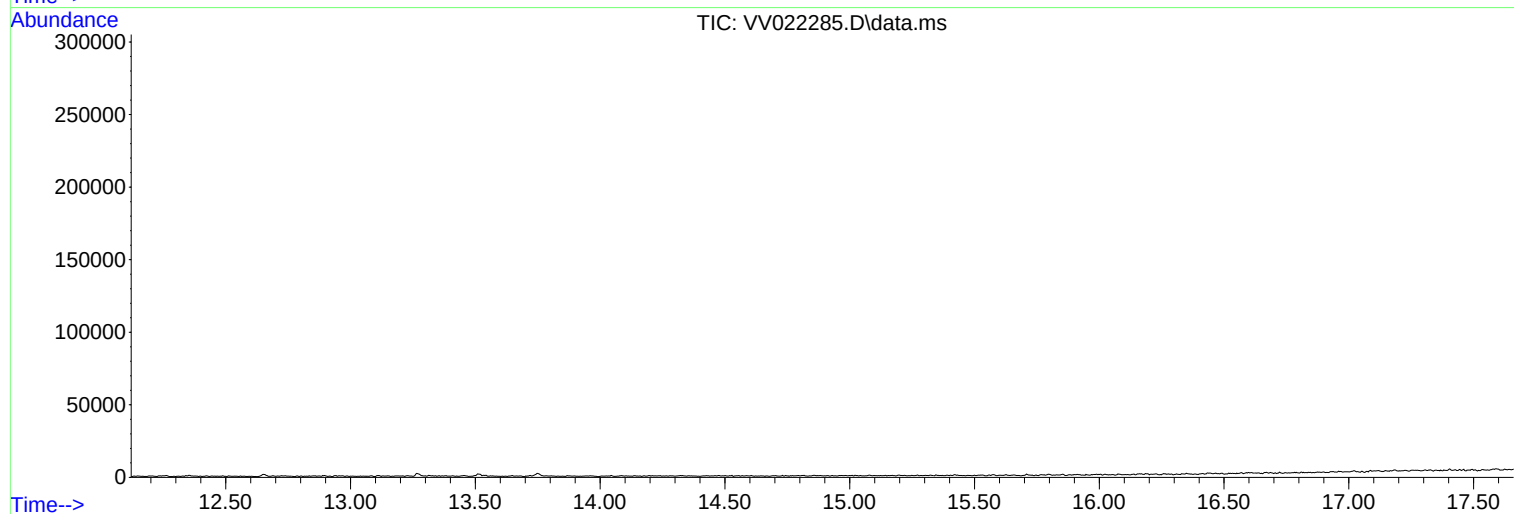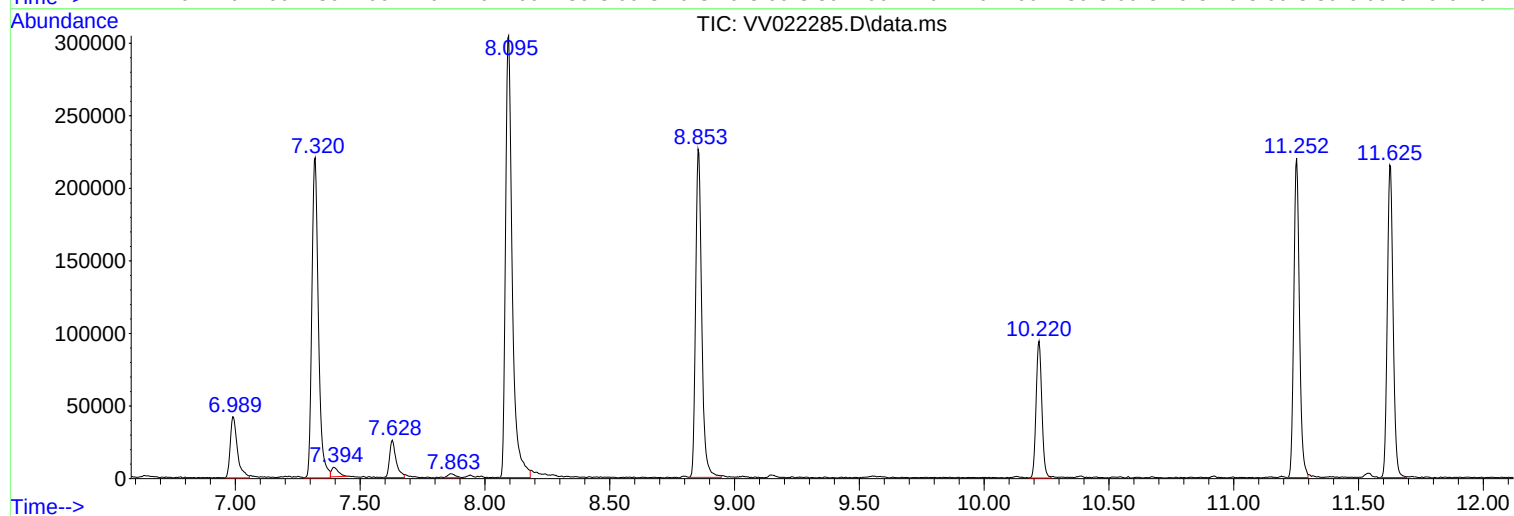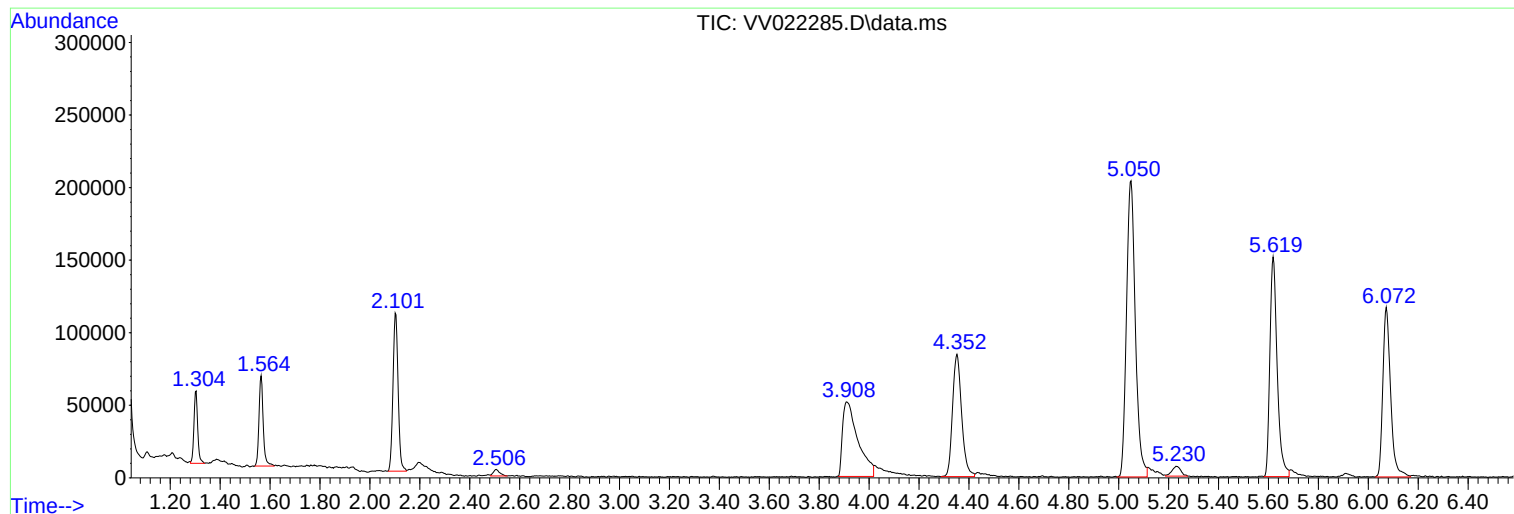

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022285.D
Acq On : 23 Sep 2021 15:43
Operator : SY/MD
Sample : M3878-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022285.D
Acq On : 23 Sep 2021 15:43
Operator : SY/MD
Sample : M3878-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
