

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022287.D
 Acq On : 23 Sep 2021 16:32
 Operator : SY/MD
 Sample : M3814-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6X6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022287.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	55270	56565	10.66%	1.352%
2	1.564	156	163	174	rVB	59787	70006	13.19%	1.673%
3	2.105	319	331	342	rBV	110601	164470	31.00%	3.931%
4	2.162	343	349	357	rVB	6040	8849	1.67%	0.211%
5	3.879	871	883	918	rBV	75568	204182	38.48%	4.880%
6	4.352	1013	1030	1052	rBV	86129	213346	40.21%	5.099%
7	5.050	1230	1247	1269	rBV3	199653	502074	94.62%	12.000%
8	5.619	1412	1424	1444	rBV	163134	331856	62.54%	7.932%
9	5.706	1447	1451	1465	rVB5	4877	8134	1.53%	0.194%
10	6.072	1552	1565	1583	rBV2	117652	245384	46.25%	5.865%
11	6.992	1839	1851	1864	rBV	42101	78891	14.87%	1.886%
12	7.320	1942	1953	1973	rBV	222064	406054	76.53%	9.705%
13	7.629	2037	2049	2066	rBV2	24920	48763	9.19%	1.165%
14	8.088	2181	2192	2218	rBV	296606	530614	100.00%	12.682%
15	8.252	2236	2243	2259	rVB8	6488	12765	2.41%	0.305%
16	8.854	2417	2430	2455	rBV	244865	420823	79.31%	10.058%
17	10.220	2841	2855	2868	rBV	91732	148811	28.05%	3.557%
18	11.252	3163	3176	3193	rBV	247201	379876	71.59%	9.079%
19	11.625	3281	3292	3314	rBV	218701	352524	66.44%	8.426%




Sum of corrected areas: 4183987

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022287.D
Acq On : 23 Sep 2021 16:32
Operator : SY/MD
Sample : M3814-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

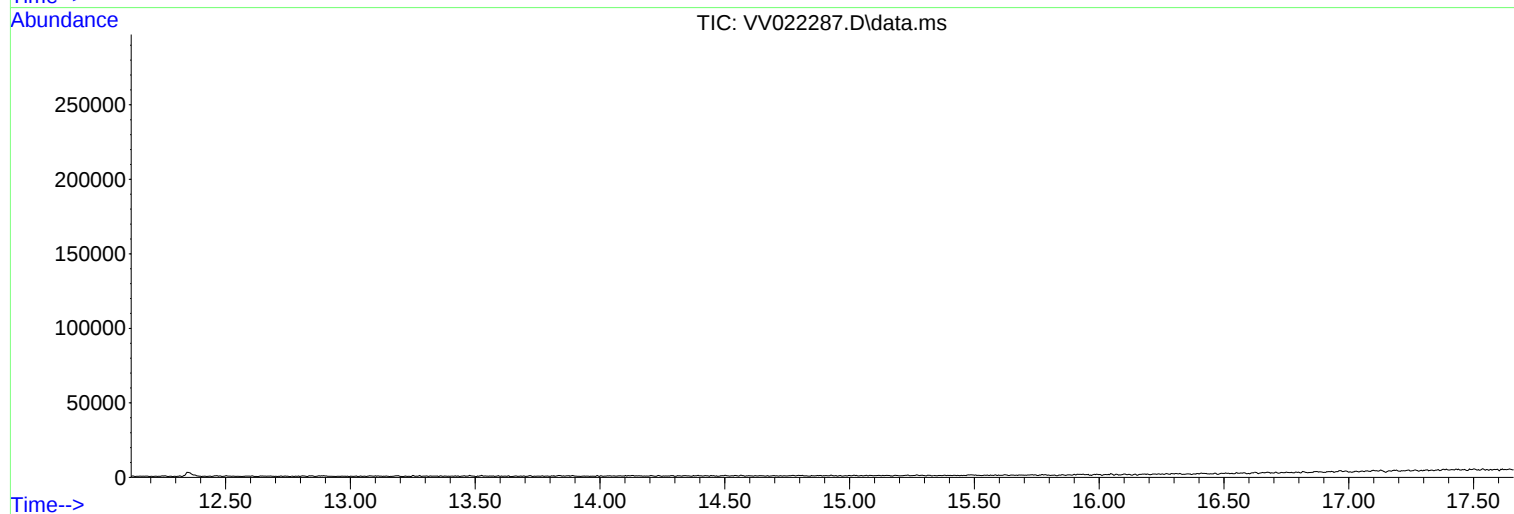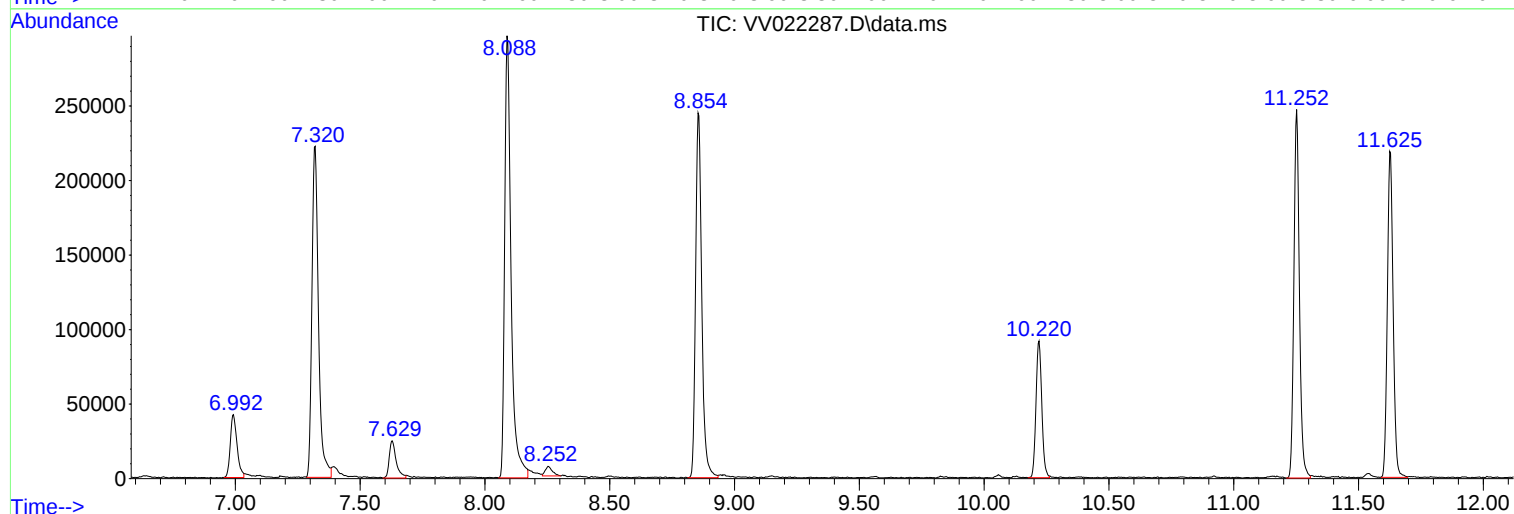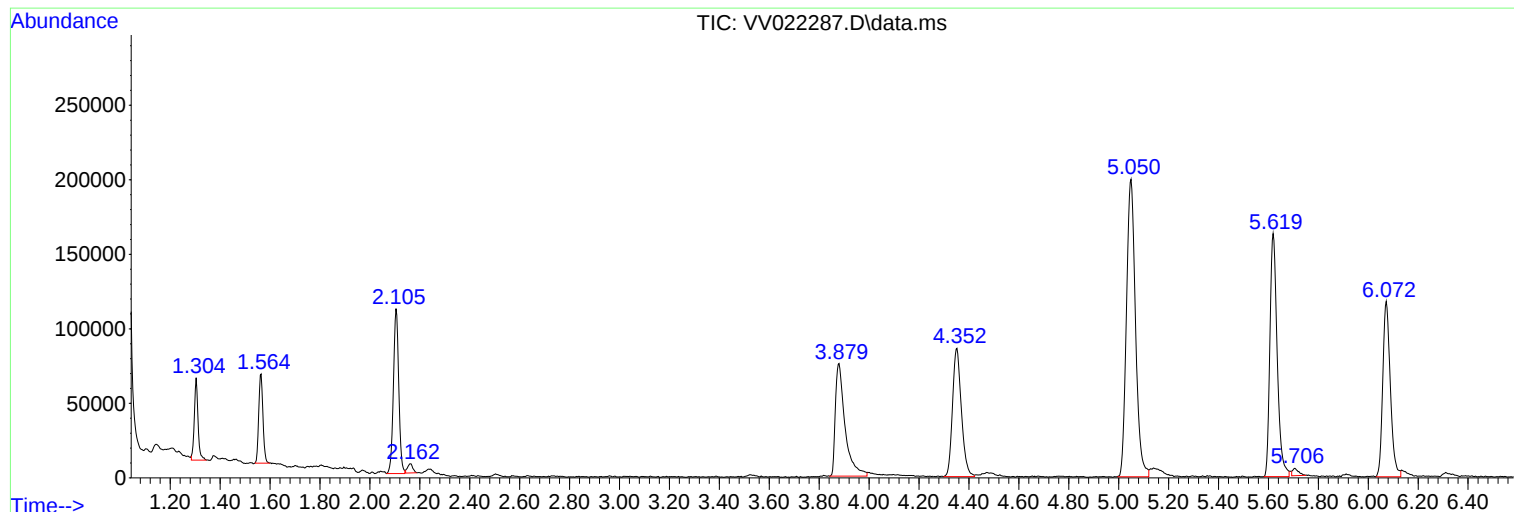

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022287.D
Acq On : 23 Sep 2021 16:32
Operator : SY/MD
Sample : M3814-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022287.D
Acq On : 23 Sep 2021 16:32
Operator : SY/MD
Sample : M3814-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6X6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
