

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022288.D
 Acq On : 23 Sep 2021 16:54
 Operator : SY/MD
 Sample : M3814-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6X7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022288.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	53080	55278	10.23%	1.348%
2	1.564	155	163	174	rVB	60572	69855	12.92%	1.704%
3	2.105	321	331	343	rBV	106810	161572	29.89%	3.941%
4	2.162	343	349	357	rVB	7771	10242	1.89%	0.250%
5	3.879	873	883	913	rBV	76299	200323	37.06%	4.886%
6	4.355	1015	1031	1050	rBV	85161	212980	39.40%	5.195%
7	5.053	1232	1248	1281	rBV2	198256	507484	93.87%	12.377%
8	5.622	1413	1425	1462	rBV	140832	300228	55.54%	7.323%
9	6.075	1553	1566	1590	rBV	116845	248590	45.98%	6.063%
10	6.297	1627	1635	1656	rBV5	9040	20930	3.87%	0.510%
11	6.992	1841	1851	1869	rBV2	42323	81678	15.11%	1.992%
12	7.320	1942	1953	1971	rBV	223411	401275	74.23%	9.787%
13	7.400	1971	1978	1991	rVB4	7269	15758	2.91%	0.384%
14	7.628	2041	2049	2072	rBV	25055	44985	8.32%	1.097%
15	8.091	2181	2193	2223	rBV	307732	540600	100.00%	13.185%
16	8.252	2235	2243	2258	rVB7	6293	11518	2.13%	0.281%
17	8.857	2420	2431	2453	rBV	221911	368507	68.17%	8.988%
18	10.220	2844	2855	2870	rBV2	94664	148986	27.56%	3.634%
19	11.252	3163	3176	3196	rBV	217609	340644	63.01%	8.308%
20	11.628	3281	3293	3314	rBV	221402	351784	65.07%	8.580%
21	12.349	3508	3517	3526	rBV7	4797	6844	1.27%	0.167%




Sum of corrected areas: 4100061

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022288.D
Acq On : 23 Sep 2021 16:54
Operator : SY/MD
Sample : M3814-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6X7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

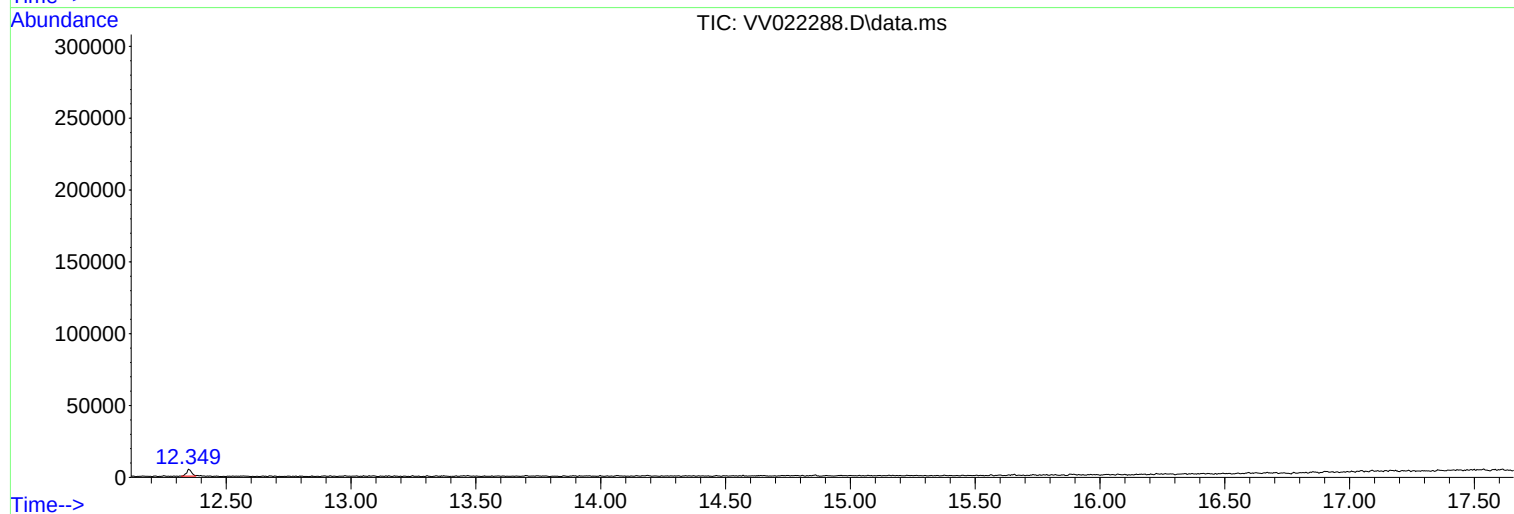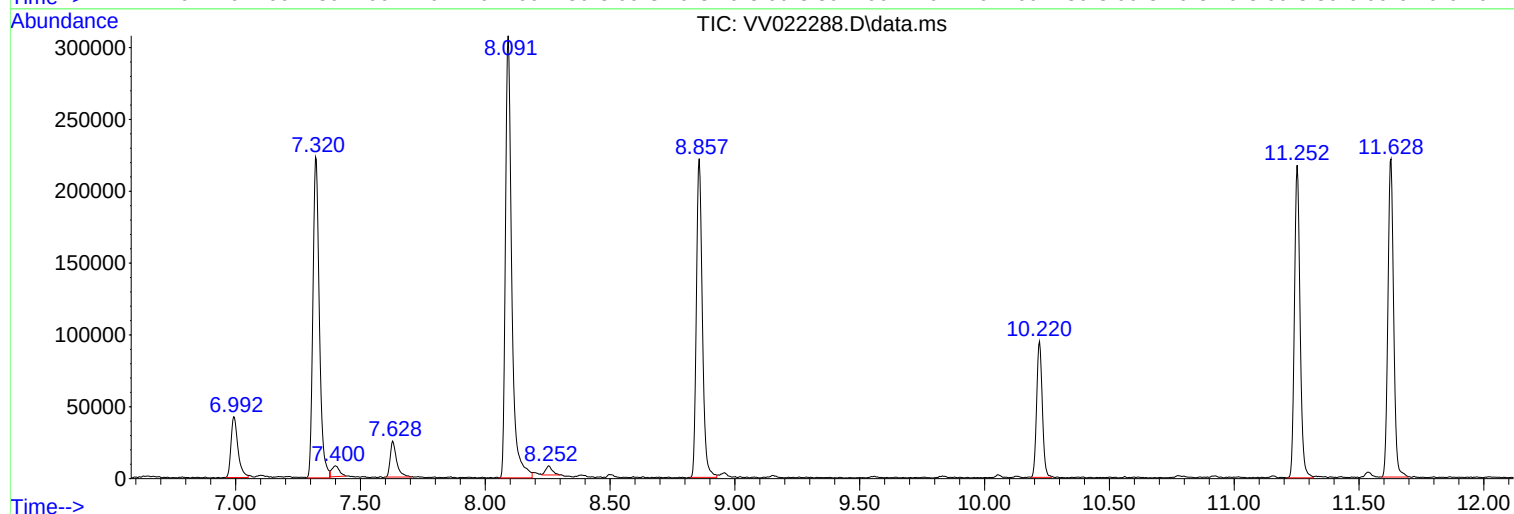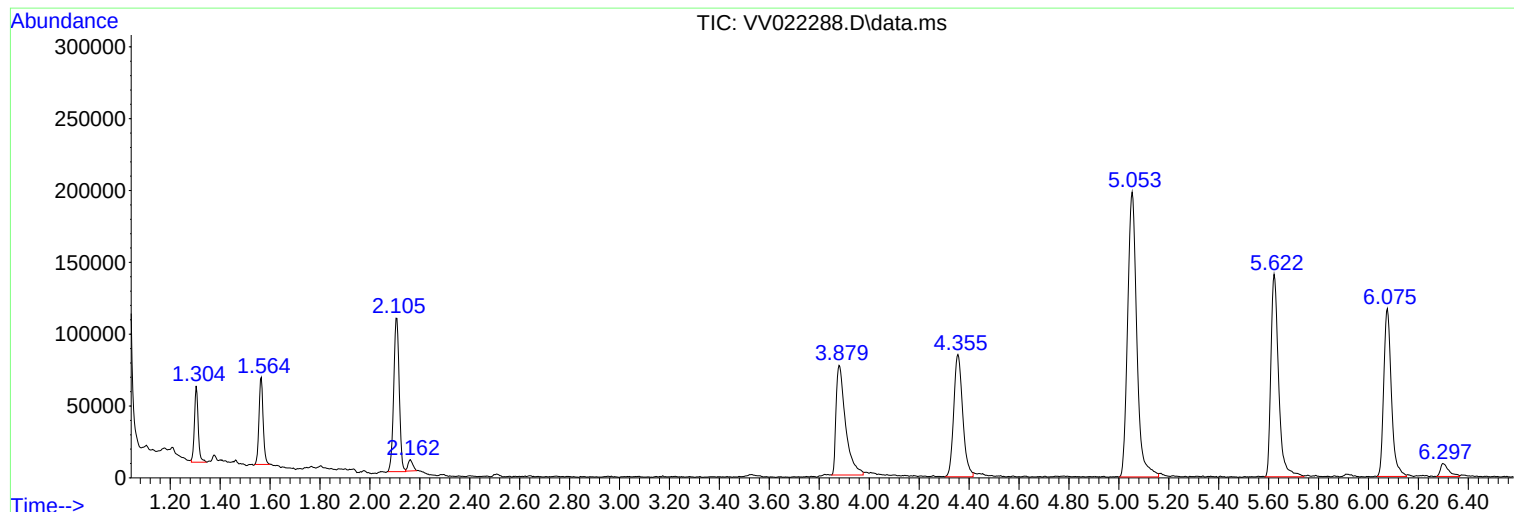

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022288.D
Acq On : 23 Sep 2021 16:54
Operator : SY/MD
Sample : M3814-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6X7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022288.D
Acq On : 23 Sep 2021 16:54
Operator : SY/MD
Sample : M3814-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6X7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
