

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022289.D
 Acq On : 23 Sep 2021 17:18
 Operator : SY/MD
 Sample : M3814-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6Y0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022289.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	91	rBV2	48088	62012	12.36%	1.578%
2	1.565	156	163	177	rBV	60105	69220	13.79%	1.761%
3	2.105	320	331	342	rBV	94830	138491	27.59%	3.524%
4	2.175	343	353	385	rVB	21308	54530	10.86%	1.388%
5	2.664	488	505	522	rBV4	3521	12199	2.43%	0.310%
6	3.687	809	823	839	rBV5	7076	18686	3.72%	0.476%
7	3.889	874	886	912	rBV	68163	195741	39.00%	4.981%
8	4.352	1009	1030	1051	rBV2	76894	194365	38.73%	4.946%
9	5.050	1228	1247	1268	rBV2	184114	460905	91.83%	11.729%
10	5.619	1413	1424	1442	rBV	143445	295376	58.85%	7.517%
11	6.072	1550	1565	1586	rBV	108961	228044	45.44%	5.803%
12	6.542	1698	1711	1717	rBV9	3061	6405	1.28%	0.163%
13	6.992	1840	1851	1869	rBV3	39134	75745	15.09%	1.928%
14	7.320	1940	1953	1974	rBV	201765	370771	73.88%	9.435%
15	7.625	2037	2048	2066	rBV	22567	43796	8.73%	1.114%
16	8.092	2183	2193	2218	rBV	274209	501888	100.00%	12.772%
17	8.854	2419	2430	2457	rBV	218332	379836	75.68%	9.666%
18	10.217	2842	2854	2868	rBV	84739	137139	27.32%	3.490%
19	11.252	3164	3176	3198	rBV	214725	336730	67.09%	8.569%
20	11.535	3254	3264	3277	rBV2	11307	21138	4.21%	0.538%
21	11.628	3281	3293	3311	rVV	201366	326678	65.09%	8.313%




Sum of corrected areas: 3929695

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022289.D
Acq On : 23 Sep 2021 17:18
Operator : SY/MD
Sample : M3814-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

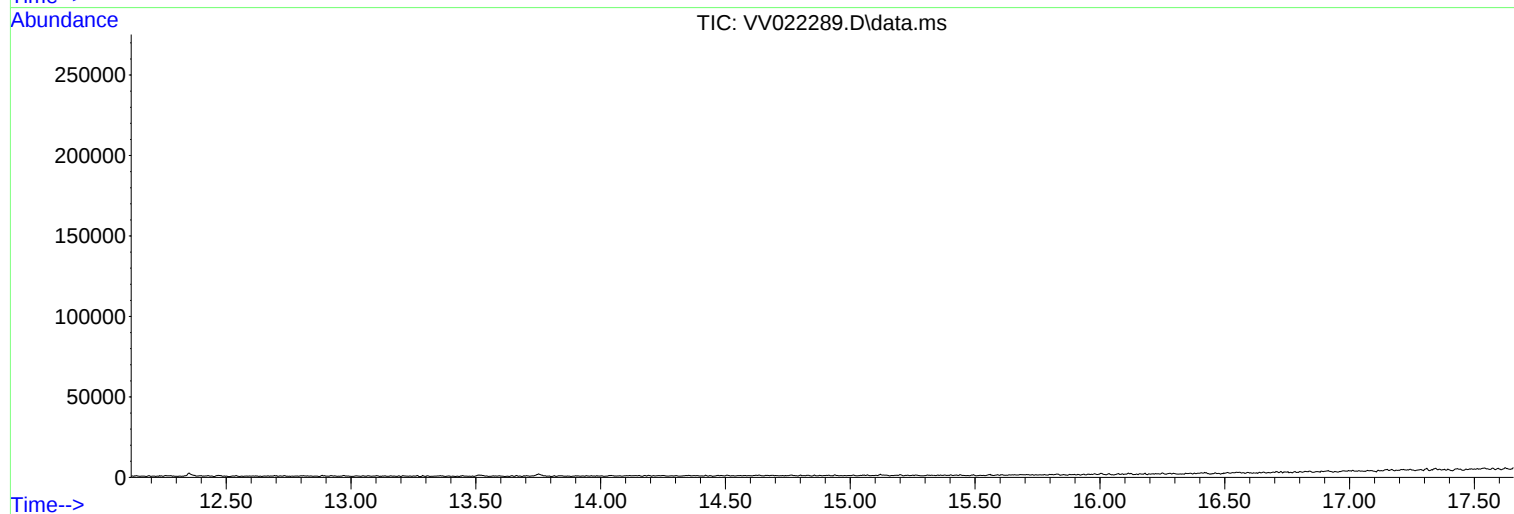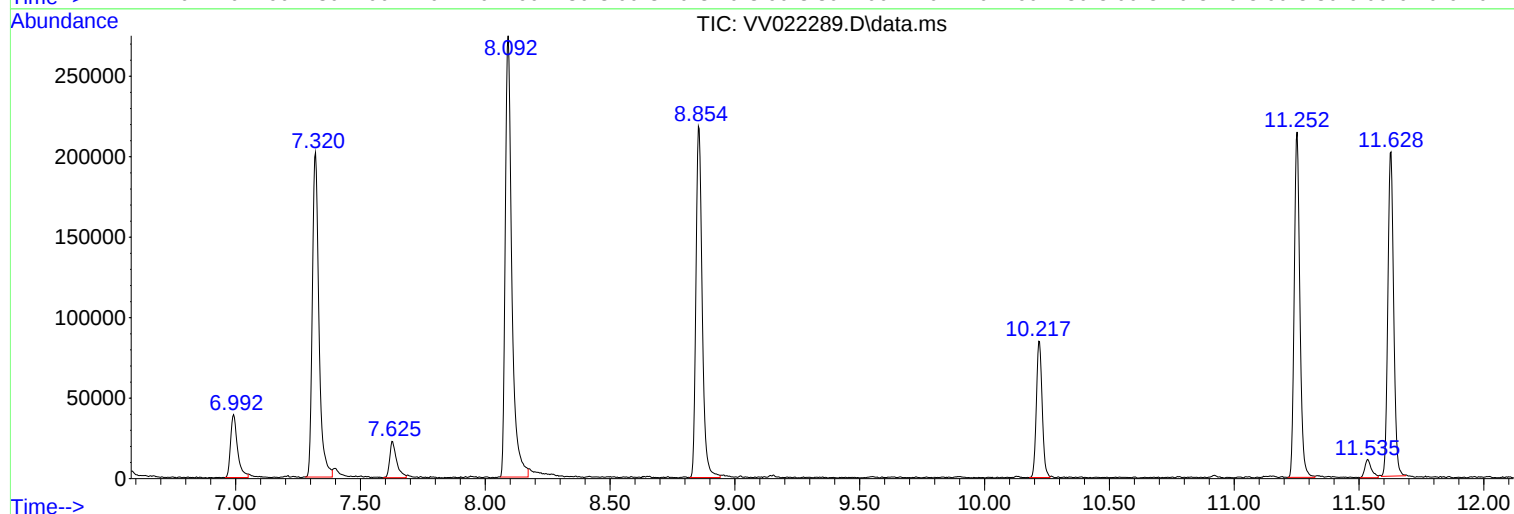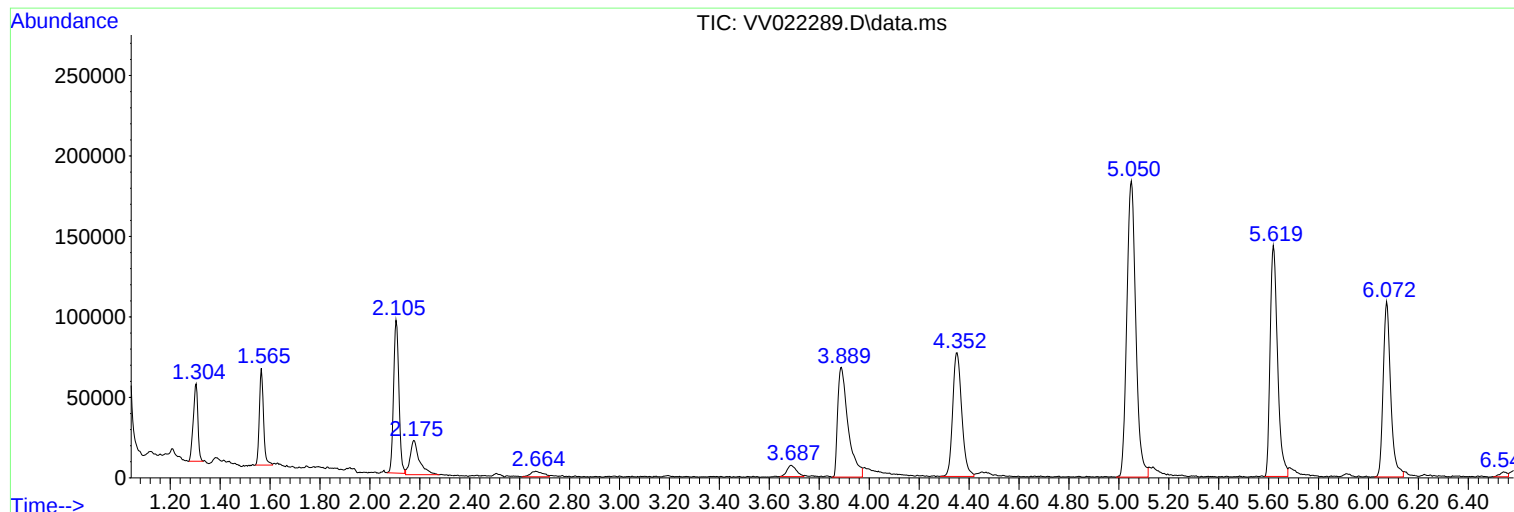

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022289.D
Acq On : 23 Sep 2021 17:18
Operator : SY/MD
Sample : M3814-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022289.D
Acq On : 23 Sep 2021 17:18
Operator : SY/MD
Sample : M3814-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------