

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022292.D
 Acq On : 23 Sep 2021 18:32
 Operator : SY/MD
 Sample : M3873-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7Y7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022292.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	35	39	46	rBV	6996	10437	1.96%	0.273%
2	1.301	76	81	99	rVB	46412	50602	9.52%	1.325%
3	1.410	111	115	125	rVB2	6671	7876	1.48%	0.206%
4	1.565	155	163	173	rBV	57372	67610	12.73%	1.770%
5	2.102	321	330	343	rBV	97978	137373	25.86%	3.597%
6	2.265	370	381	394	rVB5	3692	9638	1.81%	0.252%
7	3.912	879	893	941	rBV	48145	226740	42.68%	5.936%
8	4.352	1014	1030	1057	rBV	77236	192981	36.32%	5.052%
9	5.047	1228	1246	1273	rBV2	185582	460038	86.59%	12.044%
10	5.175	1273	1286	1300	rVB2	4290	12822	2.41%	0.336%
11	5.619	1411	1424	1444	rBV	134359	276277	52.00%	7.233%
12	6.072	1551	1565	1583	rBV2	109084	225140	42.38%	5.894%
13	6.992	1838	1851	1871	rBV	38404	74941	14.11%	1.962%
14	7.317	1941	1952	1976	rBV	198547	364347	68.58%	9.539%
15	7.629	2039	2049	2074	rBV2	21371	42186	7.94%	1.104%
16	8.095	2183	2194	2225	rBV	277926	531279	100.00%	13.909%
17	8.854	2419	2430	2461	rBV	204821	355186	66.85%	9.299%
18	10.220	2844	2855	2869	rBV	88802	141207	26.58%	3.697%
19	11.252	3165	3176	3194	rBV	196804	309616	58.28%	8.106%
20	11.628	3281	3293	3314	rBV	200105	323298	60.85%	8.464%




Sum of corrected areas: 3819594

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022292.D
Acq On : 23 Sep 2021 18:32
Operator : SY/MD
Sample : M3873-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

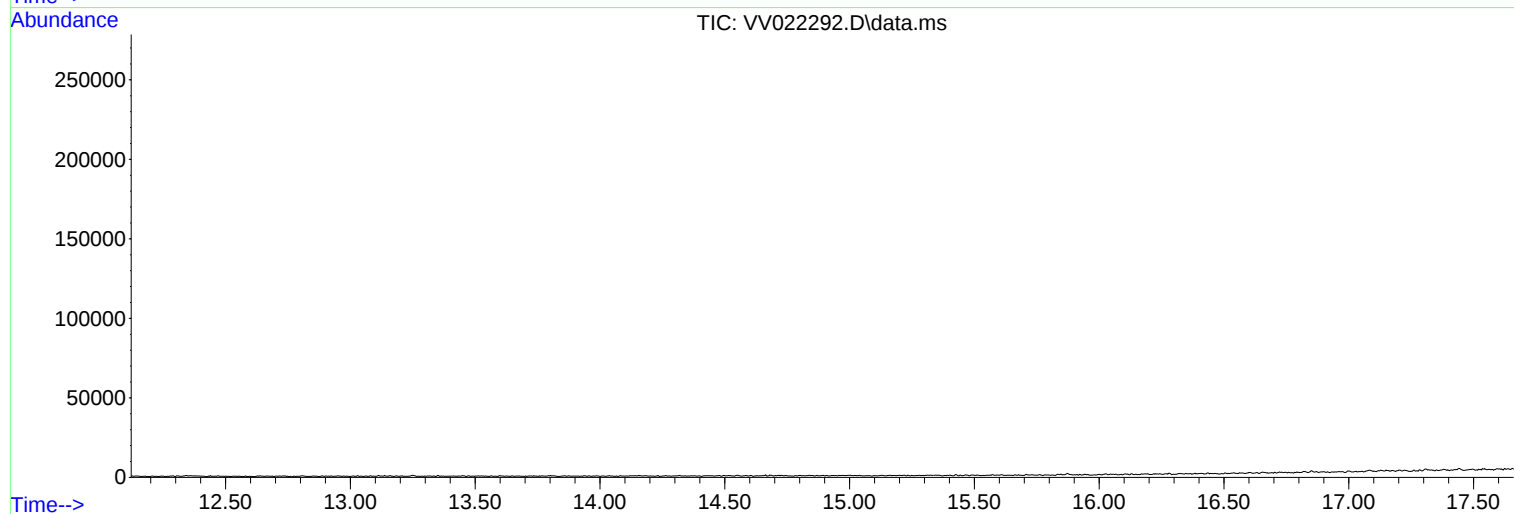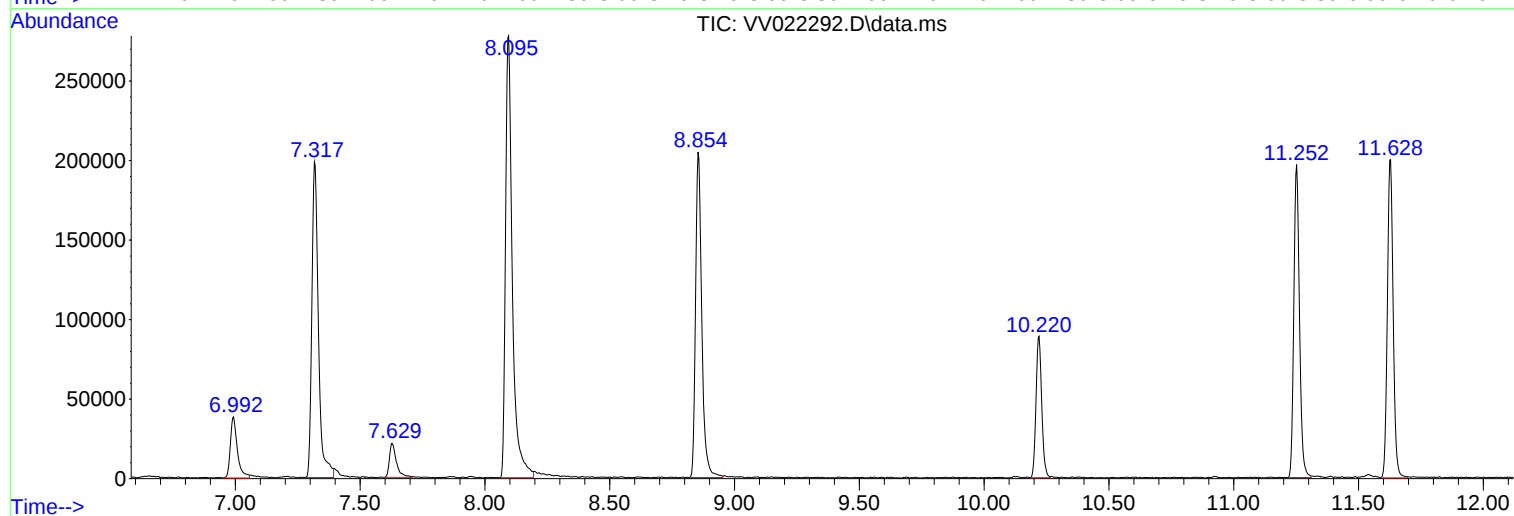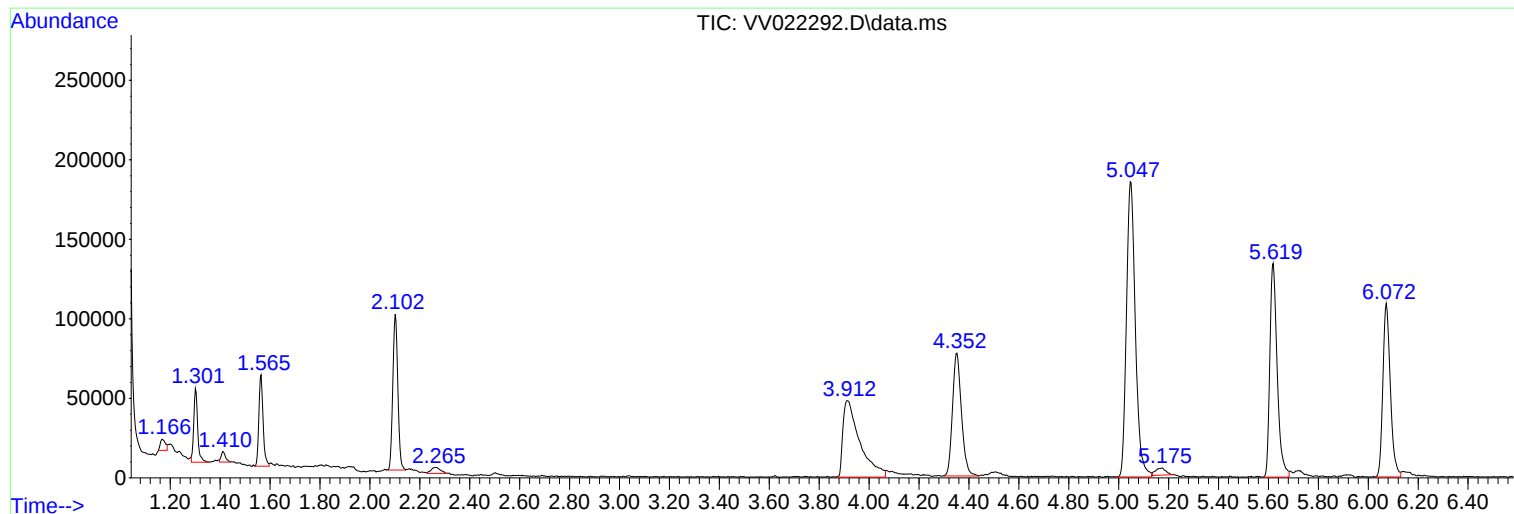

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022292.D
Acq On : 23 Sep 2021 18:32
Operator : SY/MD
Sample : M3873-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022292.D
Acq On : 23 Sep 2021 18:32
Operator : SY/MD
Sample : M3873-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------