

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022299.D
 Acq On : 23 Sep 2021 21:47
 Operator : SY/MD
 Sample : VV0923WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK210

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022299.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	23	28	43	rVB	9035	13349	2.50%	0.349%
2	1.301	75	81	93	rVB	47706	49436	9.26%	1.292%
3	1.564	156	163	178	rBV	56489	65332	12.24%	1.708%
4	2.101	318	330	343	rBV	96817	144060	26.99%	3.766%
5	2.220	359	367	370	rBV5	3735	5467	1.02%	0.143%
6	3.918	883	895	938	rBV	43340	208835	39.13%	5.459%
7	4.352	1012	1030	1053	rBV2	79757	201227	37.70%	5.260%
8	5.050	1232	1247	1270	rBV2	191376	471852	88.41%	12.335%
9	5.140	1273	1275	1294	rVB7	6050	11330	2.12%	0.296%
10	5.619	1410	1424	1441	rBV	133189	275653	51.65%	7.206%
11	6.072	1549	1565	1583	rBV	108608	228040	42.73%	5.961%
12	6.992	1839	1851	1874	rBV	38002	76156	14.27%	1.991%
13	7.320	1938	1953	1973	rBV	201506	374243	70.12%	9.783%
14	7.629	2040	2049	2072	rBV2	21731	44313	8.30%	1.158%
15	8.095	2184	2194	2223	rBV	277300	533722	100.00%	13.952%
16	8.857	2417	2431	2450	rBV	203228	350897	65.75%	9.173%
17	10.220	2842	2855	2867	rBV	88938	142180	26.64%	3.717%
18	11.252	3164	3176	3195	rBV	193756	307287	57.57%	8.033%
19	11.628	3280	3293	3312	rBV	202701	322071	60.34%	8.419%




Sum of corrected areas: 3825450

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022299.D
Acq On : 23 Sep 2021 21:47
Operator : SY/MD
Sample : VV0923WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK210

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

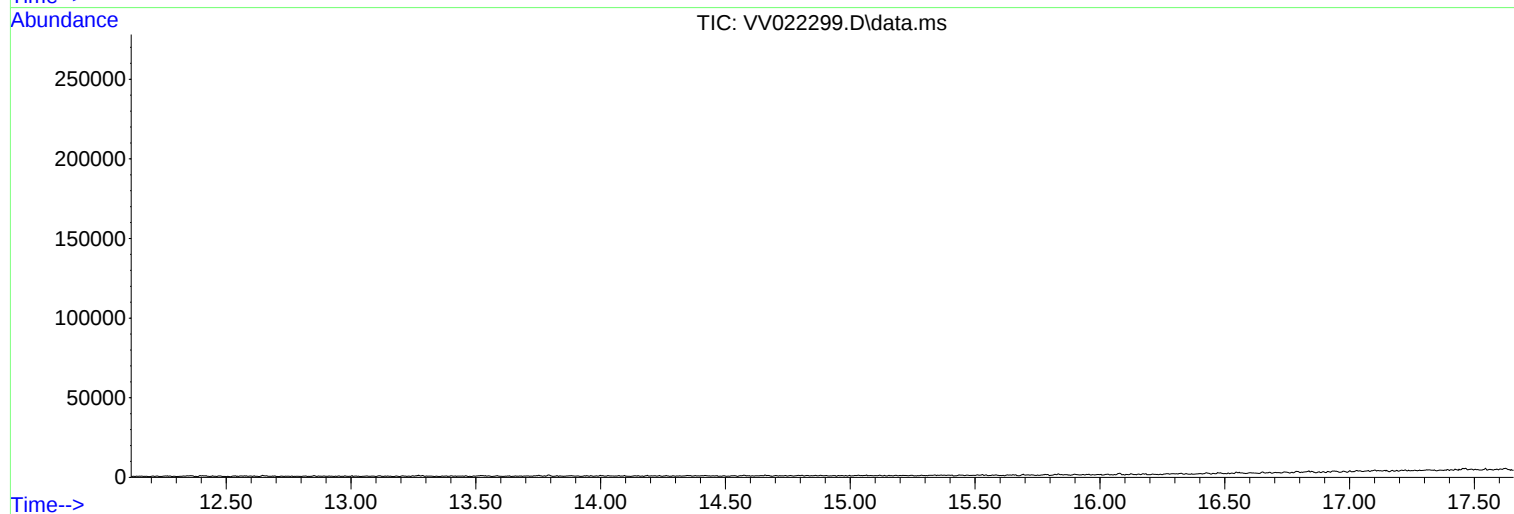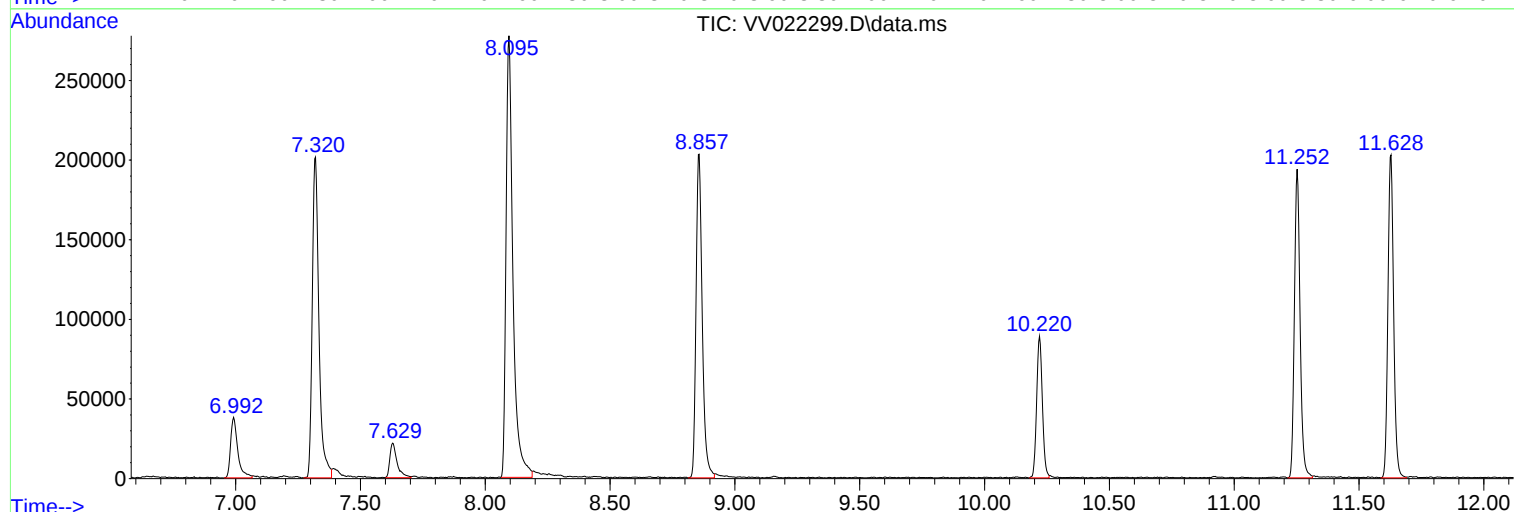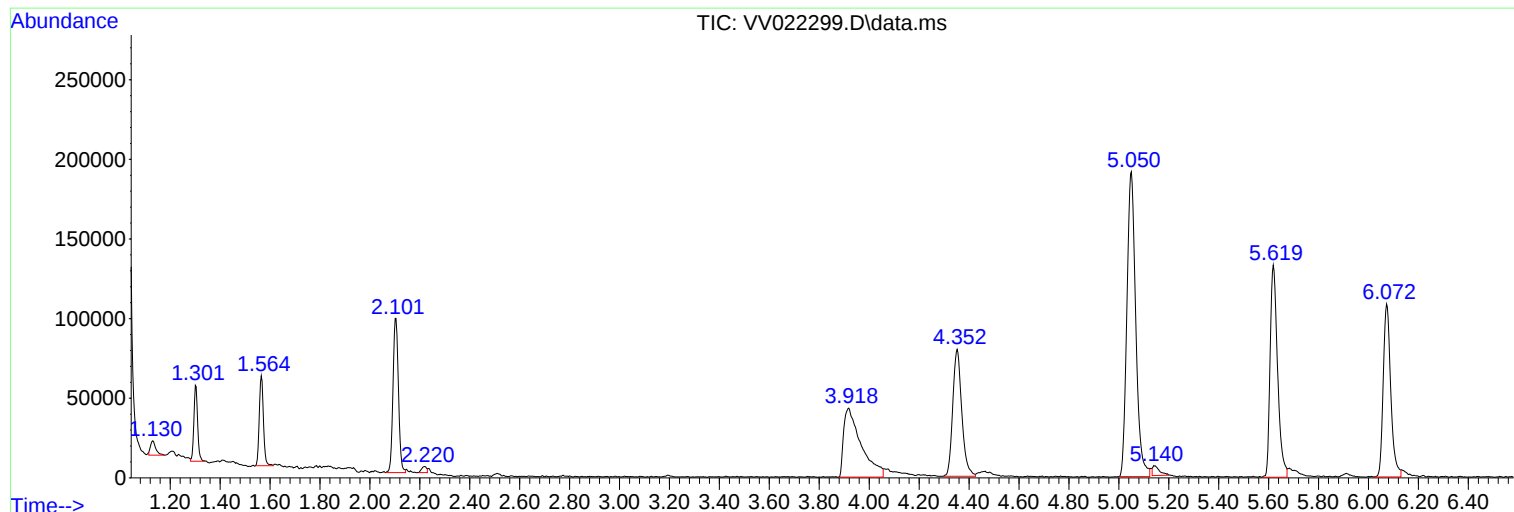

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022299.D
Acq On : 23 Sep 2021 21:47
Operator : SY/MD
Sample : VV0923WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK210

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022299.D
Acq On : 23 Sep 2021 21:47
Operator : SY/MD
Sample : VV0923WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK210

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
