

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022301.D
 Acq On : 23 Sep 2021 22:36
 Operator : SY/MD
 Sample : M3878-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2P4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	92	rVB	48028	48965	8.76%	1.234%
2	1.564	155	163	174	rBV	61999	72137	12.91%	1.818%
3	2.101	319	330	344	rBV	104655	150829	26.99%	3.801%
4	2.503	445	455	468	rBV4	6451	11329	2.03%	0.286%
5	3.912	879	893	927	rBV	48949	209167	37.43%	5.272%
6	4.349	1013	1029	1049	rBV2	81928	205735	36.81%	5.185%
7	5.047	1230	1246	1274	rBV3	198423	500869	89.63%	12.624%
8	5.619	1410	1424	1445	rBV	136415	282241	50.50%	7.113%
9	6.072	1551	1565	1587	rBV	112858	243576	43.59%	6.139%
10	6.992	1841	1851	1872	rBV2	39014	75447	13.50%	1.902%
11	7.320	1936	1953	1971	rBV	212639	385810	69.04%	9.724%
12	7.397	1971	1977	1986	rVB2	6413	11464	2.05%	0.289%
13	7.628	2037	2049	2066	rBV	24205	46085	8.25%	1.162%
14	8.095	2183	2194	2221	rBV	291356	558844	100.00%	14.085%
15	8.853	2419	2430	2459	rBV	208609	358447	64.14%	9.034%
16	10.220	2844	2855	2870	rBV	91729	145318	26.00%	3.663%
17	11.252	3165	3176	3193	rBV	195697	312252	55.87%	7.870%
18	11.532	3256	3263	3280	rBV3	6637	12039	2.15%	0.303%
19	11.625	3280	3292	3313	rVV	209231	337156	60.33%	8.497%




Sum of corrected areas: 3967710

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022301.D
Acq On : 23 Sep 2021 22:36
Operator : SY/MD
Sample : M3878-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2P4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

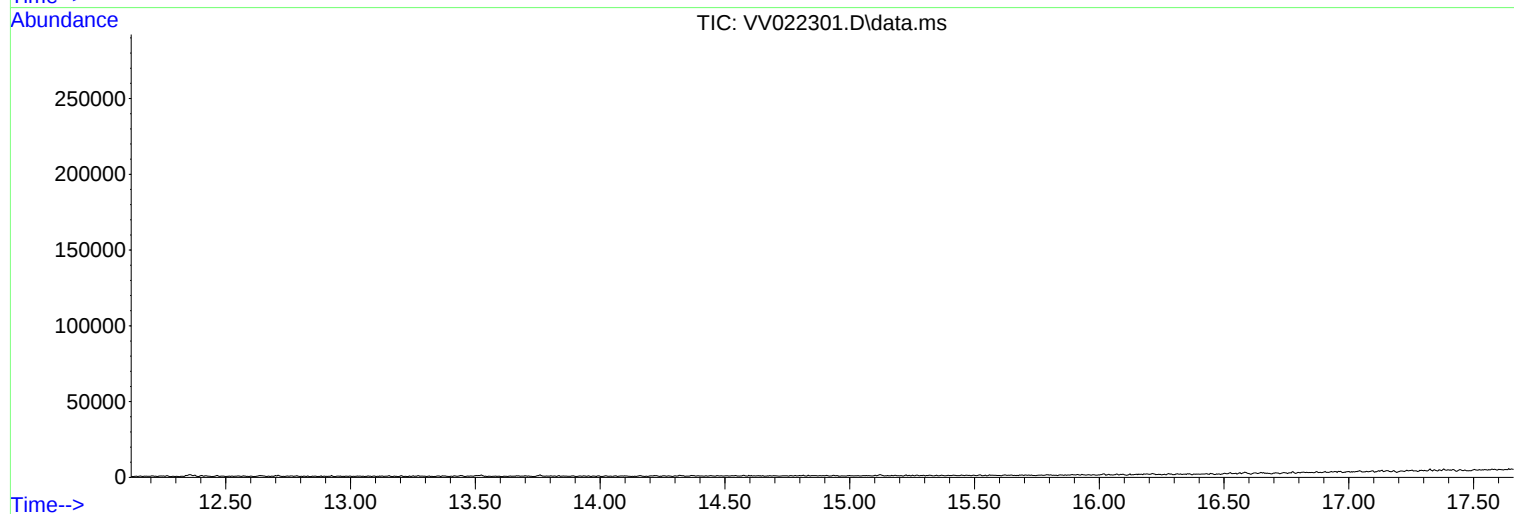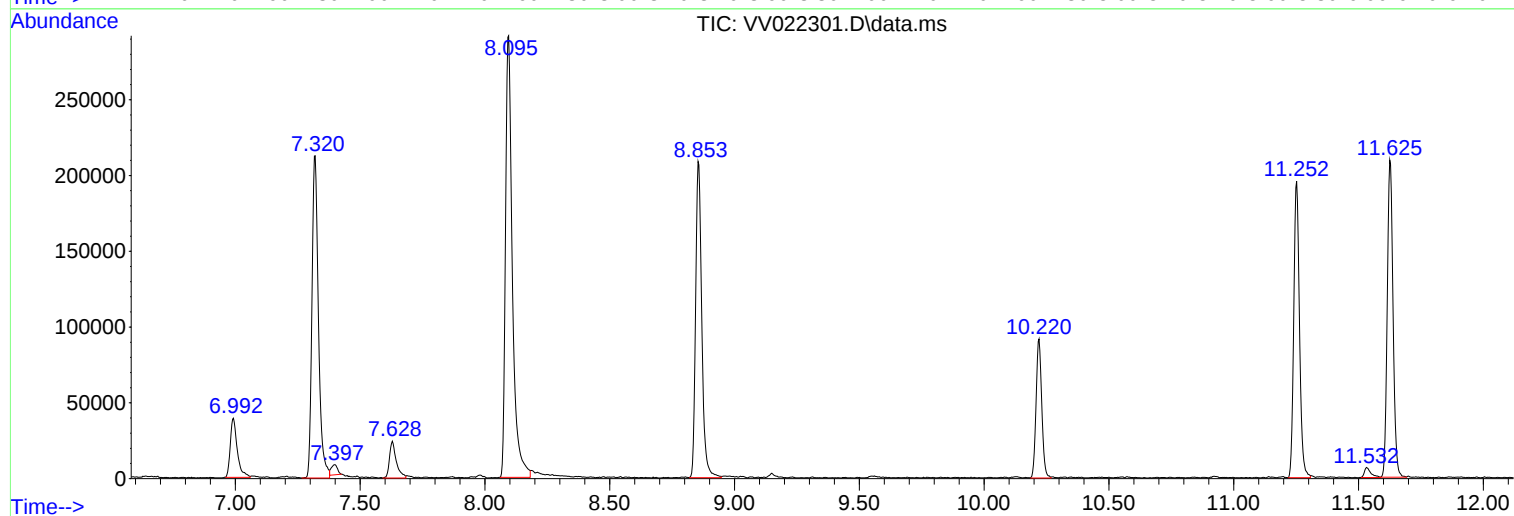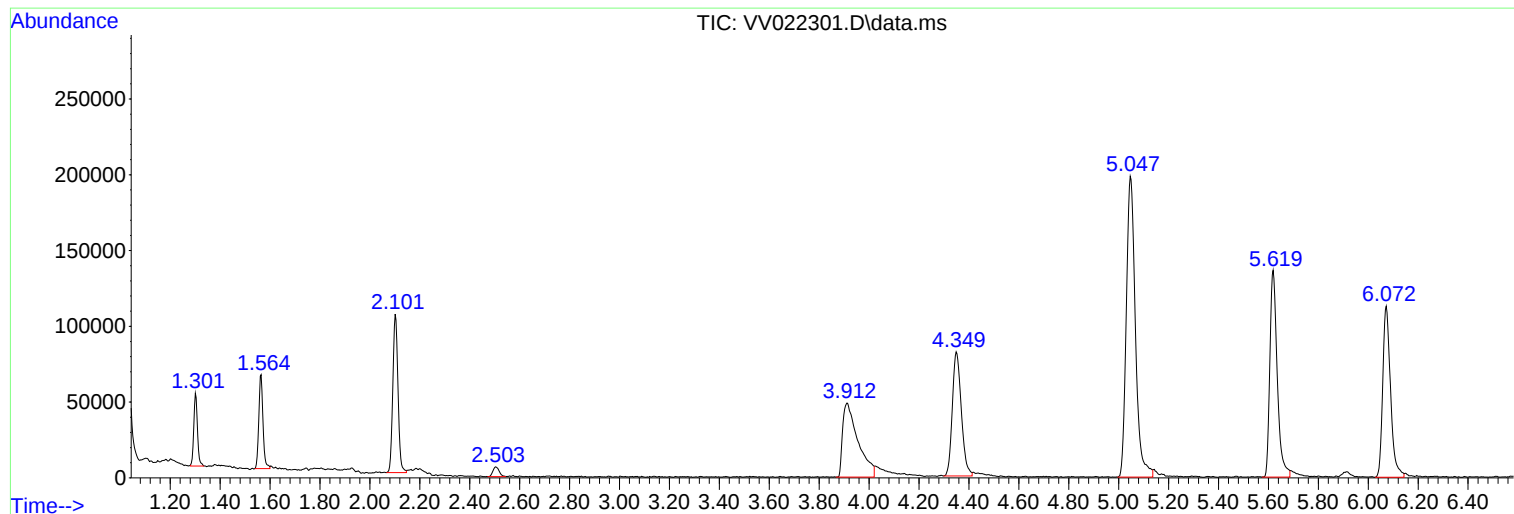

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022301.D
Acq On : 23 Sep 2021 22:36
Operator : SY/MD
Sample : M3878-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2P4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
Data File : VV022301.D
Acq On : 23 Sep 2021 22:36
Operator : SY/MD
Sample : M3878-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2P4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
