

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV092321\  
 Data File : VV022304.D  
 Acq On : 23 Sep 2021 23:50  
 Operator : SY/MD  
 Sample : M3878-06  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 35 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EW2N4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092321WMA.M  
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022304.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.304       | 76            | 82          | 88           | rVB      | 45913          | 45101         | 8.16%           | 1.164%        |
| 2         | 1.565       | 156           | 163         | 177          | rVB      | 57294          | 67397         | 12.19%          | 1.739%        |
| 3         | 2.105       | 320           | 331         | 346          | rBV      | 101108         | 145390        | 26.29%          | 3.751%        |
| 4         | 2.217       | 358           | 366         | 376          | rVB7     | 3892           | 7538          | 1.36%           | 0.194%        |
| 5         | 3.905       | 880           | 891         | 936          | rBV      | 55248          | 222524        | 40.24%          | 5.741%        |
| 6         | 4.352       | 1013          | 1030        | 1051         | rBV      | 81571          | 204637        | 37.00%          | 5.279%        |
| 7         | 5.050       | 1231          | 1247        | 1270         | rBV2     | 191443         | 477903        | 86.42%          | 12.329%       |
| 8         | 5.619       | 1413          | 1424        | 1448         | rBV      | 132465         | 275578        | 49.83%          | 7.109%        |
| 9         | 6.072       | 1551          | 1565        | 1599         | rBV2     | 114188         | 242953        | 43.93%          | 6.268%        |
| 10        | 6.992       | 1840          | 1851        | 1871         | rBV2     | 37934          | 74630         | 13.49%          | 1.925%        |
| 11        | 7.320       | 1940          | 1953        | 1973         | rBV      | 206824         | 379715        | 68.66%          | 9.796%        |
| 12        | 7.629       | 2039          | 2049        | 2070         | rBV      | 22310          | 45420         | 8.21%           | 1.172%        |
| 13        | 8.092       | 2182          | 2193        | 2223         | rBV      | 295761         | 553029        | 100.00%         | 14.267%       |
| 14        | 8.854       | 2416          | 2430        | 2450         | rBV      | 204141         | 347818        | 62.89%          | 8.973%        |
| 15        | 10.220      | 2843          | 2855        | 2868         | rBV      | 92408          | 147097        | 26.60%          | 3.795%        |
| 16        | 11.252      | 3165          | 3176        | 3195         | rBV      | 188468         | 302487        | 54.70%          | 7.804%        |
| 17        | 11.535      | 3255          | 3264        | 3271         | rBV2     | 4433           | 6891          | 1.25%           | 0.178%        |
| 18        | 11.628      | 3281          | 3293        | 3309         | rBV      | 206919         | 330132        | 59.70%          | 8.517%        |




Sum of corrected areas: 3876240

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV092321\  
Data File : VV022304.D  
Acq On : 23 Sep 2021 23:50  
Operator : SY/MD  
Sample : M3878-06  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 35 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
EW2N4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092321WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

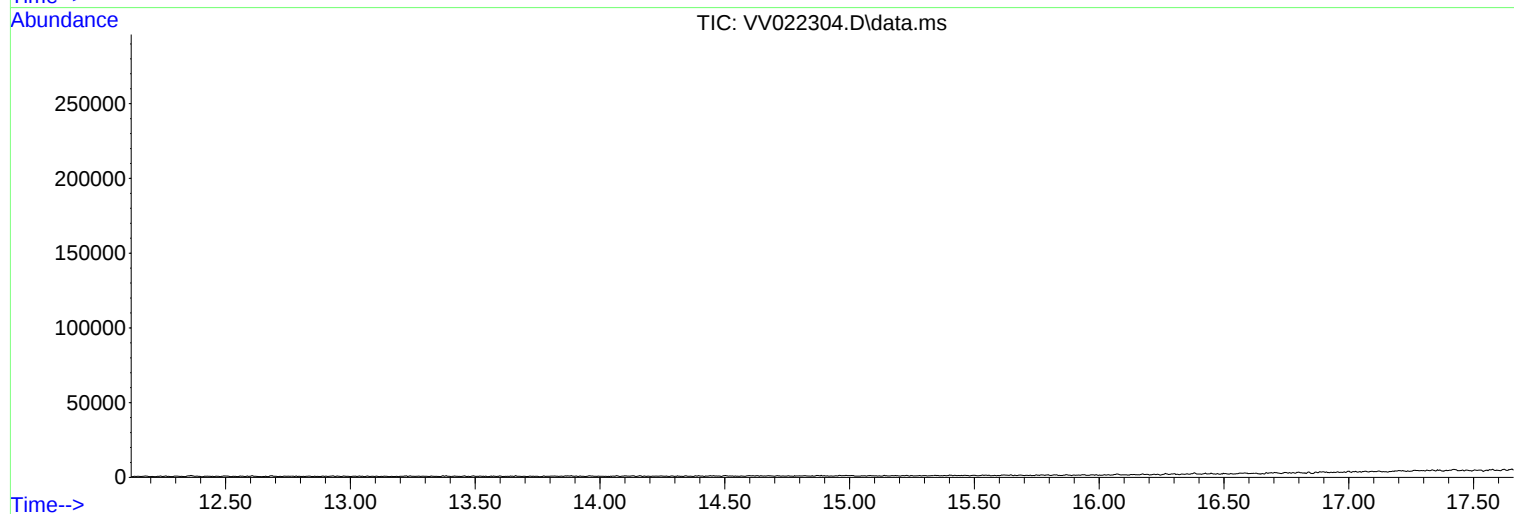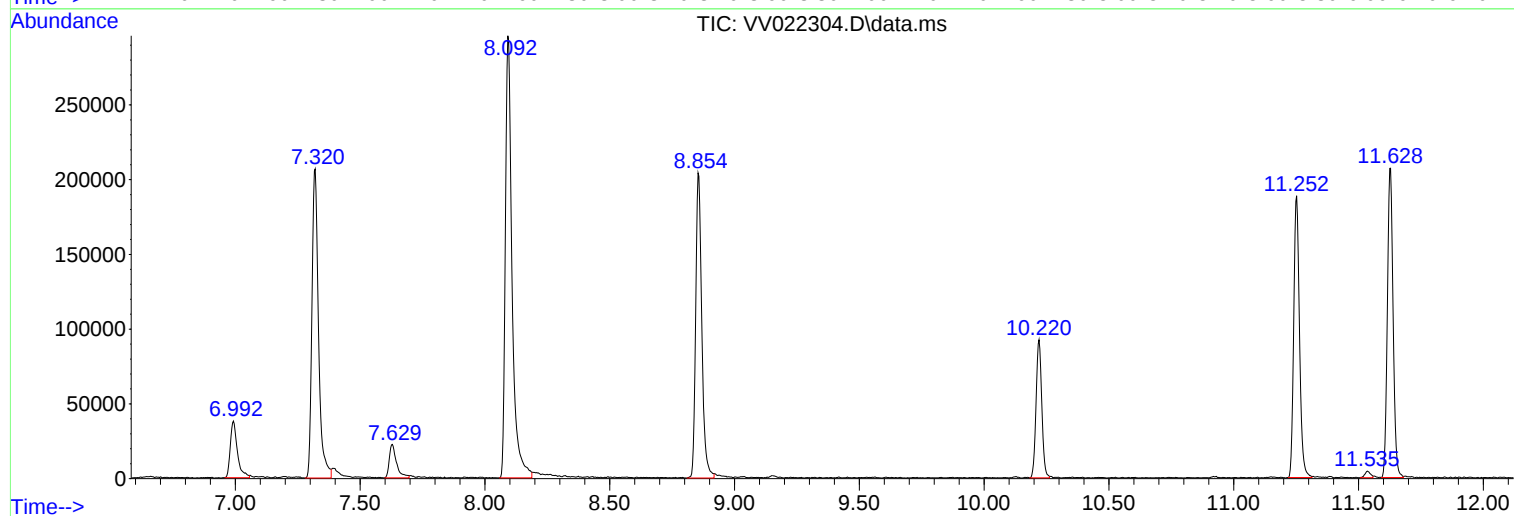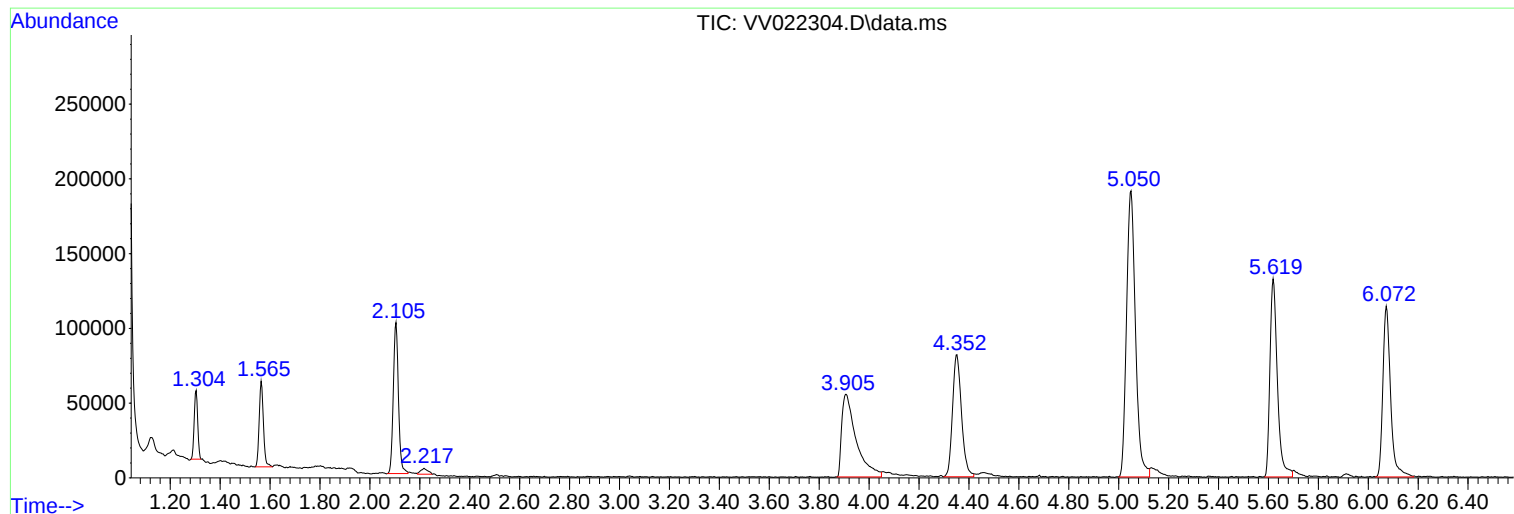

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV092321\  
Data File : VV022304.D  
Acq On : 23 Sep 2021 23:50  
Operator : SY/MD  
Sample : M3878-06  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 35 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
EW2N4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092321WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV092321\  
Data File : VV022304.D  
Acq On : 23 Sep 2021 23:50  
Operator : SY/MD  
Sample : M3878-06  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 35 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
EW2N4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR092321WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----