

m/z	Abundance
36.00	913.0
37.00	4534.0
38.00	4297.0
39.00	1905.0
40.10	223.0
42.00	103.0
44.00	814.0
45.00	848.0
46.00	197.0
47.00	1229.0
48.00	657.0
49.00	4112.0
50.00	17880.0
51.00	5453.0
52.00	325.0
53.20	144.0
55.00	309.0
56.00	1425.0
57.00	2760.0
58.00	110.0
60.00	935.0
61.00	4785.0
62.00	4862.0
63.00	3959.0
64.00	533.0
65.00	843.0
66.00	143.0
66.90	237.0
68.00	9716.0
69.00	9827.0
70.00	830.0
72.00	613.0
73.00	4336.0
74.00	16400.0
75.00	47696.0
76.00	3897.0
77.10	661.0
77.90	376.0
78.90	3536.0
80.00	1092.0
80.90	3610.0
81.90	818.0
83.00	122.0
86.00	165.0
87.00	4454.0
88.00	4013.0
90.90	380.0
92.00	2872.0
93.00	4317.0
94.00	11788.0
95.00	94280.0
96.00	6446.0
97.00	180.0
103.90	476.0
104.80	183.0
105.90	504.0
106.70	141.0
112.10	113.0
112.70	131.0
114.70	128.0
115.80	392.0
116.90	717.0
117.90	506.0
118.90	612.0
125.90	117.0
127.90	390.0
128.70	153.0
129.90	402.0
131.00	226.0
134.90	241.0
136.90	212.0
140.90	1029.0
141.80	145.0
142.90	1290.0
144.80	288.0
146.00	148.0
147.90	204.0
154.90	329.0
157.10	123.0
158.90	160.0
171.00	122.0
172.00	1214.0
173.00	1215.0
174.00	81168.0
175.00	5582.0
176.00	77576.0
177.00	4981.0
178.10	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
40.00	240.0
41.50	107.0
43.90	273.0
44.70	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	910.0
37.00	4629.0
38.00	4268.0
39.00	1917.0
40.00	234.0
44.00	735.0
45.10	890.0
46.00	196.0
47.00	1157.0
48.00	664.0
49.00	4100.0
50.00	17728.0
51.00	5494.0
52.00	319.0
53.10	117.0
55.00	334.0
56.00	1373.0
57.00	2811.0
58.10	119.0
60.00	944.0
61.00	4669.0
62.00	4684.0
63.00	3903.0
64.00	545.0
65.00	883.0
66.00	152.0
66.90	314.0
68.00	9770.0
69.00	9841.0
70.00	883.0
72.00	565.0
73.00	4409.0
74.00	16019.0
75.00	46376.0
76.00	3856.0
77.10	661.0
77.90	429.0
78.90	3602.0
79.90	1025.0
80.90	3508.0
81.90	873.0
83.00	115.0
85.90	185.0
87.00	4414.0
87.90	3871.0
90.90	437.0
92.00	2718.0
93.00	4316.0
94.00	11489.0
95.00	93024.0
96.00	6495.0
97.00	203.0
103.90	474.0
104.80	190.0
105.80	467.0
106.80	141.0
110.80	102.0
112.00	132.0
112.70	159.0
115.80	376.0
116.90	733.0
117.90	484.0
118.90	593.0
125.90	113.0
127.90	308.0
128.80	182.0
129.90	377.0
131.00	180.0
134.90	183.0
136.90	198.0
140.90	1054.0
141.80	131.0
142.90	1217.0
144.70	293.0
145.90	145.0
147.90	231.0
148.80	120.0
152.90	107.0
154.90	277.0
157.00	138.0
158.90	137.0
170.90	119.0
172.00	1100.0
173.00	1118.0
174.00	77640.0
175.00	5535.0
176.00	74176.0
177.00	4840.0
178.10	145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB205

m/z	Abundance
36.00	786.0
37.00	4079.0
38.00	3896.0
39.00	1769.0
40.10	208.0
44.00	857.0
45.00	786.0
46.00	175.0
47.00	1106.0
48.00	620.0
49.00	3668.0
50.00	16008.0
51.00	4920.0
52.10	282.0
53.20	146.0
55.00	263.0
56.00	1364.0
57.00	2395.0
58.00	118.0
60.00	820.0
61.00	4398.0
62.00	4475.0
63.00	3597.0
64.00	450.0
65.00	699.0
67.10	184.0
68.00	8496.0
69.00	8865.0
70.00	770.0
71.90	625.0
73.10	3957.0
74.00	15116.0
75.00	43800.0
76.00	3669.0
77.00	566.0
77.80	345.0
78.90	3170.0
80.00	1075.0
80.90	3389.0
81.90	722.0
82.80	122.0
86.10	171.0
87.00	3905.0
88.00	3841.0
90.90	335.0
92.00	2699.0
93.00	3855.0
94.00	10799.0
95.00	86776.0
96.00	5780.0
97.00	146.0
103.90	397.0
104.90	172.0
105.90	501.0
106.70	160.0
112.80	104.0
114.80	130.0
115.80	331.0
116.90	678.0
117.90	442.0
118.90	561.0
127.90	418.0
128.60	139.0
129.10	102.0
129.90	402.0
130.90	196.0
134.80	227.0
136.90	180.0
141.00	919.0
141.80	157.0
142.90	1293.0
144.80	238.0
145.90	125.0
147.90	184.0
149.80	117.0
154.90	365.0
157.10	132.0
158.80	156.0
170.90	124.0
172.00	1183.0
173.00	1191.0
174.00	76848.0
175.00	5173.0
176.00	73744.0
177.00	4619.0
178.10	138.0



Instrument :
MSVOA_V
ClientSampleId :
BFB205

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092321\
 Data File : VV022272.D
 Acq On : 23 Sep 2021 09:37
 Operator : SY/MD
 Sample : BFB205
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB205

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Sep 28 01:24:48 2021

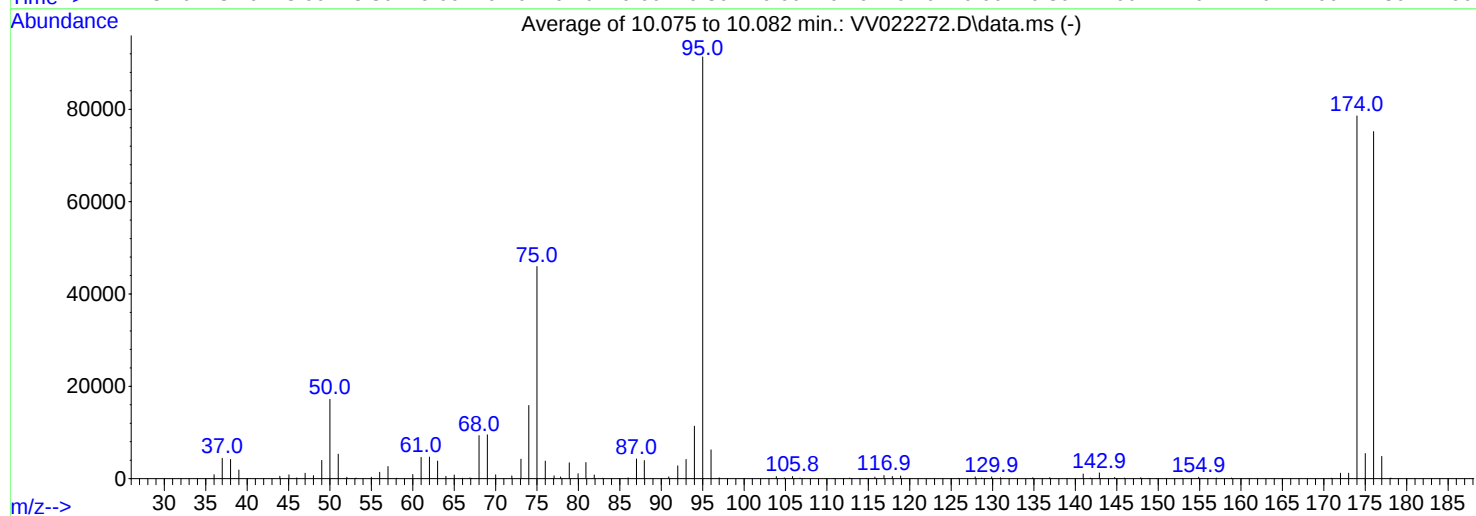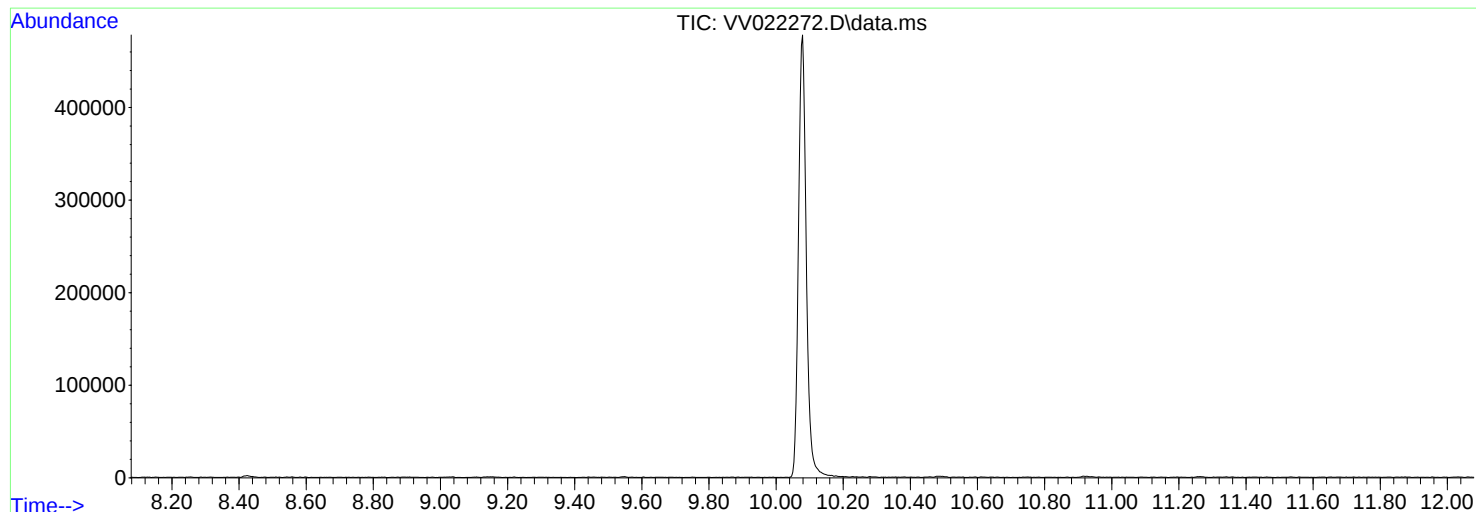

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	17205	PASS
75	95	30	80	50.3	45957	PASS
95	95	100	100	100.0	91360	PASS
96	95	5	9	6.8	6240	PASS
173	174	0.00	2	1.5	1175	PASS
174	95	50	120	86.0	78552	PASS
175	174	5	9	6.9	5430	PASS
176	174	95	105	95.7	75165	PASS
177	176	5	10	6.4	4813	PASS