

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092418\
 Data File : VV007824.D
 Acq On : 24 Sep 2018 18:33
 Operator : SY/MD
 Sample : J5012-05DL 100X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C08L3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	64	72	87	rVB	61311	66539	6.99%	1.203%
2	1.586	147	154	165	rBV	66513	74436	7.82%	1.346%
3	2.135	315	325	336	rBV	156695	223021	23.44%	4.033%
4	3.624	785	788	792	rVB	150	106	0.01%	0.002%
5	3.952	874	890	927	rBV	40319	115993	12.19%	2.097%
6	4.254	982	984	988	rVB2	367	267	0.03%	0.005%
7	4.283	989	993	996	rVV	247	178	0.02%	0.003%
8	4.338	1006	1010	1013	rBV	141	118	0.01%	0.002%
9	4.409	1013	1032	1052	rBV	93294	220392	23.16%	3.985%
10	4.556	1075	1078	1082	rBV	205	140	0.01%	0.003%
11	4.634	1100	1102	1109	rVB	121	106	0.01%	0.002%
12	5.007	1215	1218	1224	rVB	124	103	0.01%	0.002%
13	5.103	1230	1248	1279	rBV2	225133	548510	57.64%	9.918%
14	5.347	1321	1324	1326	rBV	151	122	0.01%	0.002%
15	5.412	1340	1344	1348	rBV	107	104	0.01%	0.002%
16	5.518	1375	1377	1381	rVB2	199	126	0.01%	0.002%
17	5.547	1381	1386	1392	rBV	122	161	0.02%	0.003%
18	5.672	1410	1425	1457	rBV	208812	415652	43.68%	7.516%
19	5.900	1494	1496	1504	rVB2	290	194	0.02%	0.004%
20	5.955	1504	1513	1522	rBV4	2332	4292	0.45%	0.078%
21	6.126	1552	1566	1594	rBV	121531	246747	25.93%	4.462%
22	6.245	1600	1603	1605	rBV2	390	325	0.03%	0.006%
23	6.257	1605	1607	1615	rVV2	412	326	0.03%	0.006%
24	6.299	1616	1620	1623	rVB	203	121	0.01%	0.002%
25	6.344	1628	1634	1638	rBV	214	182	0.02%	0.003%
26	6.454	1663	1668	1671	rBV2	176	132	0.01%	0.002%
27	7.035	1837	1849	1870	rBV	65407	115034	12.09%	2.080%
28	7.174	1887	1892	1896	rVV2	403	413	0.04%	0.007%
29	7.193	1896	1898	1900	rVB	230	111	0.01%	0.002%
30	7.257	1912	1918	1921	rBV	95	95	0.01%	0.002%
31	7.363	1938	1951	1973	rBV	268357	472793	49.69%	8.549%
32	7.576	2015	2017	2021	rVB2	379	192	0.02%	0.003%
33	7.669	2035	2046	2063	rBV2	45695	76991	8.09%	1.392%
34	7.814	2089	2091	2094	rBV2	138	109	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092418\
 Data File : VV007824.D
 Acq On : 24 Sep 2018 18:33
 Operator : SY/MD
 Sample : J5012-05DL 100X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C08L3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

35	7.846	2099	2101	2105	rVB	169	131	0.01%	0.002%
36	7.868	2105	2108	2113	rBV2	346	345	0.04%	0.006%
37	7.987	2142	2145	2151	rBV2	309	358	0.04%	0.006%
38	8.019	2151	2155	2156	rBV2	1507	1050	0.11%	0.019%
39	8.138	2181	2192	2230	rBV	131270	252310	26.51%	4.562%
40	8.415	2274	2278	2282	rBV3	279	262	0.03%	0.005%
41	8.650	2344	2351	2353	rBV	126	137	0.01%	0.002%
42	8.785	2389	2393	2401	rVB	120	162	0.02%	0.003%
43	8.900	2416	2429	2434	rBV	323387	533349	56.05%	9.644%
44	9.129	2498	2500	2504	rVB	263	183	0.02%	0.003%
45	9.180	2514	2516	2519	rBV2	337	216	0.02%	0.004%
46	9.215	2522	2527	2532	rVB	97	125	0.01%	0.002%
47	9.244	2532	2536	2539	rBV	145	119	0.01%	0.002%
48	9.408	2581	2587	2589	rBV	95	101	0.01%	0.002%
49	9.592	2636	2644	2646	rBV	291	236	0.02%	0.004%
50	9.611	2647	2650	2654	rVB2	214	158	0.02%	0.003%
51	9.650	2660	2662	2671	rVB	116	144	0.02%	0.003%
52	9.974	2760	2763	2768	rVB2	206	196	0.02%	0.004%
53	10.151	2811	2818	2823	rVB	124	147	0.02%	0.003%
54	10.267	2842	2854	2880	rBV	188867	302871	31.83%	5.477%
55	10.424	2895	2903	2905	rBV	345	266	0.03%	0.005%
56	10.440	2906	2908	2910	rVV	184	101	0.01%	0.002%
57	10.469	2914	2917	2924	rVV	181	221	0.02%	0.004%
58	10.550	2935	2942	2947	rBV	122	190	0.02%	0.003%
59	11.010	3082	3085	3090	rVV	112	106	0.01%	0.002%
60	11.231	3144	3154	3164	rVV	21587	32641	3.43%	0.590%
61	11.299	3164	3175	3203	rVB2	352306	688387	72.34%	12.447%
62	11.415	3203	3211	3215	rBV	96	125	0.01%	0.002%
63	11.682	3280	3294	3320	rBV2	394746	951575	100.00%	17.206%
64	11.826	3336	3339	3342	rBV2	153	103	0.01%	0.002%
65	11.871	3347	3353	3357	rBV2	227	230	0.02%	0.004%
66	11.916	3362	3367	3369	rBV	124	117	0.01%	0.002%
67	11.990	3386	3390	3392	rBV	248	140	0.01%	0.003%
68	12.006	3392	3395	3399	rVV	127	132	0.01%	0.002%
69	12.045	3404	3407	3412	rVB2	184	192	0.02%	0.003%
70	12.077	3413	3417	3419	rVV2	189	113	0.01%	0.002%
71	12.151	3438	3440	3443	rVB2	198	109	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092418\
 Data File : VV007824.D
 Acq On : 24 Sep 2018 18:33
 Operator : SY/MD
 Sample : J5012-05DL 100X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C08L3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis

72	12.183	3443	3450	3456	rBV	116	180	0.02%	0.003%
73	12.209	3456	3458	3461	rVB	184	119	0.01%	0.002%
74	12.338	3496	3498	3502	rVB2	282	143	0.02%	0.003%
75	12.363	3502	3506	3508	rBV	196	161	0.02%	0.003%
76	12.453	3530	3534	3537	rVB2	620	435	0.05%	0.008%
77	12.473	3537	3540	3543	rVB	170	98	0.01%	0.002%
78	12.489	3543	3545	3551	rVB2	162	136	0.01%	0.002%
79	12.524	3552	3556	3559	rVB2	163	108	0.01%	0.002%
80	12.540	3559	3561	3563	rBV	259	137	0.01%	0.002%
81	12.614	3582	3584	3586	rBV	226	118	0.01%	0.002%
82	12.659	3595	3598	3602	rBV2	196	168	0.02%	0.003%
83	12.698	3604	3610	3621	rVB4	908	1444	0.15%	0.026%
84	12.746	3621	3625	3627	rBV2	221	180	0.02%	0.003%
85	12.836	3650	3653	3655	rBV	191	123	0.01%	0.002%
86	12.878	3663	3666	3671	rBV2	160	122	0.01%	0.002%
87	12.993	3699	3702	3705	rBV	216	176	0.02%	0.003%
88	13.074	3725	3727	3731	rVB2	241	199	0.02%	0.004%
89	13.100	3731	3735	3737	rBV	249	187	0.02%	0.003%
90	13.225	3770	3774	3777	rBV2	245	251	0.03%	0.005%
91	13.315	3791	3802	3818	rVB	90085	142993	15.03%	2.586%
92	13.489	3852	3856	3860	rBV	271	333	0.03%	0.006%
93	13.800	3942	3953	3964	rBV2	19022	28500	3.00%	0.515%
94	14.071	4034	4037	4040	rVV2	181	101	0.01%	0.002%
95	14.608	4202	4204	4205	rBV2	211	97	0.01%	0.002%
96	14.858	4280	4282	4286	rBV2	331	225	0.02%	0.004%
97	14.907	4295	4297	4298	rBV2	245	111	0.01%	0.002%
98	15.042	4337	4339	4342	rBV2	308	138	0.01%	0.002%
99	15.460	4464	4469	4475	rVB4	1190	1439	0.15%	0.026%
100	15.710	4545	4547	4551	rBV4	572	449	0.05%	0.008%


Sum of corrected areas: 5530350

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092418\
Data File : VV007824.D
Acq On : 24 Sep 2018 18:33
Operator : SY/MD
Sample : J5012-05DL 100X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C08L3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

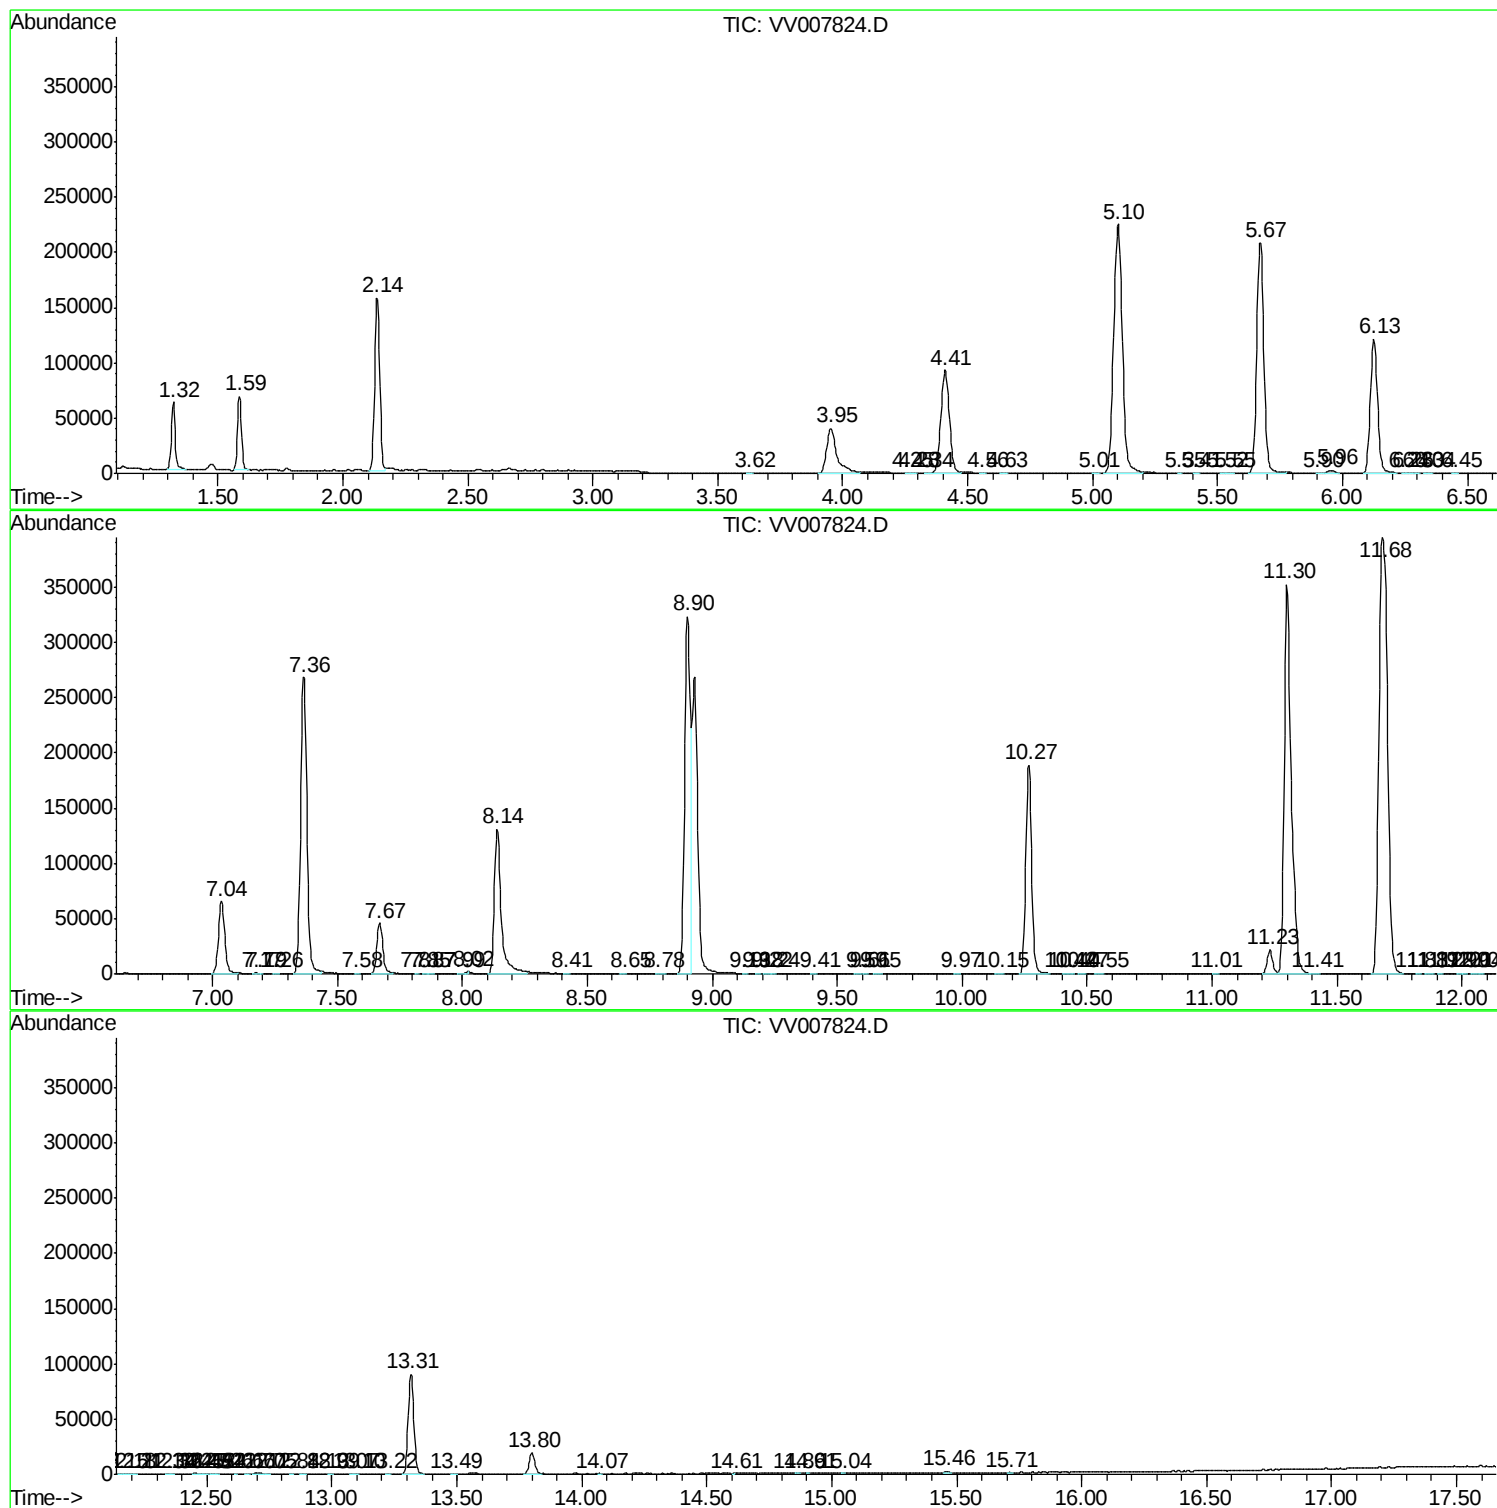

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV092418\
Data File : VV007824.D
Acq On : 24 Sep 2018 18:33
Operator : SY/MD
Sample : J5012-05DL 100X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C08L3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV092418\
Data File : VV007824.D
Acq On : 24 Sep 2018 18:33
Operator : SY/MD
Sample : J5012-05DL 100X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C08L3DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc