


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV092418\
 Data File : VV007803.D
 Acq On : 24 Sep 2018 08:57
 Operator : SY/MD
 Sample : BFB72
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB72

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092318WMA.M
 Title : VOC Analysis
 Last Update : Tue Sep 25 04:04:32 2018

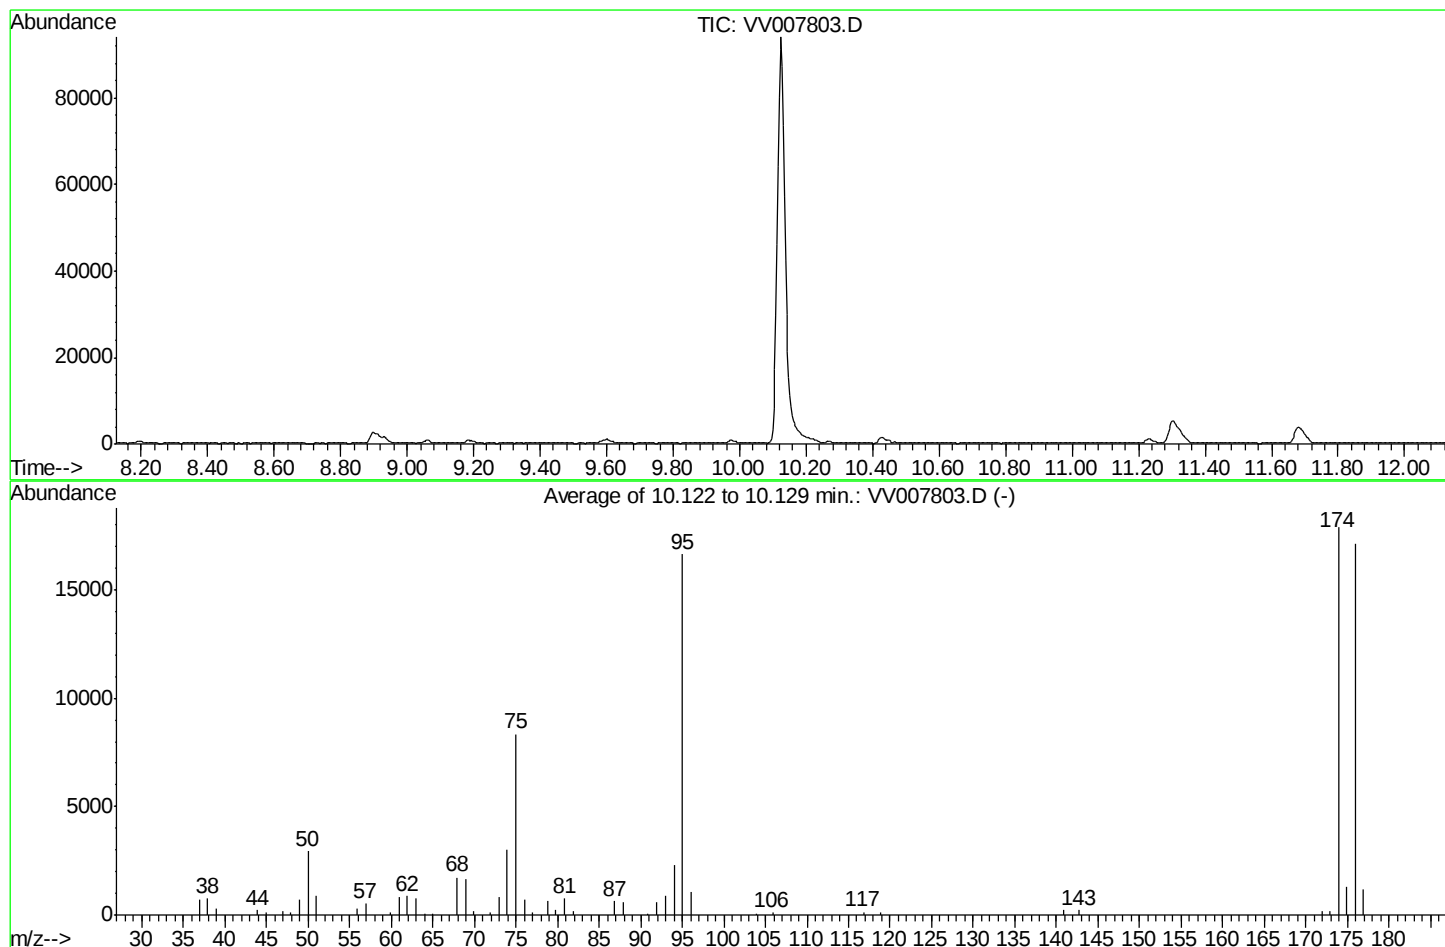

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	2951	PASS
75	95	30	80	50.2	8354	PASS
95	95	100	100	100.0	16639	PASS
96	95	5	9	6.4	1057	PASS
173	174	0.00	2	1.1	195	PASS
174	95	50	120	107.5	17885	PASS
175	174	5	9	7.3	1311	PASS
176	174	95	101	95.7	17109	PASS
177	176	5	9	7.1	1207	PASS

m/z	Abundance
43.80	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
36.90	800.0
38.00	829.0
38.90	277.0
44.00	383.0
44.90	160.0
47.00	176.0
47.90	120.0
48.90	681.0
50.00	3034.0
51.00	912.0
55.90	343.0
57.00	511.0
59.90	135.0
60.90	833.0
61.90	874.0
63.00	809.0
65.00	104.0
67.90	1712.0
69.00	1768.0
69.90	168.0
71.90	149.0
72.90	803.0
74.00	3204.0
75.00	8365.0
76.00	773.0
77.10	119.0
78.80	658.0
79.80	240.0
80.90	681.0
81.90	165.0
86.90	665.0
87.90	659.0
90.90	112.0
91.90	611.0
93.00	918.0
94.00	2361.0
95.00	16856.0
96.00	1113.0
105.80	116.0
116.90	142.0
118.80	121.0
140.80	214.0
142.70	223.0
171.90	182.0
173.90	17720.0
174.90	1284.0
175.90	16904.0
176.90	1269.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
37.00	740.0
37.90	776.0
38.90	316.0
44.00	388.0
44.90	143.0
47.00	192.0
47.90	135.0
48.90	753.0
50.00	3024.0
51.00	913.0
56.00	321.0
56.90	524.0
59.90	150.0
60.90	855.0
61.90	905.0
63.00	794.0
64.00	107.0
65.00	116.0
67.90	1792.0
69.00	1706.0
69.90	168.0
71.80	144.0
72.90	837.0
74.00	3117.0
75.00	8649.0
76.00	745.0
77.10	139.0
78.90	671.0
79.80	235.0
80.90	758.0
81.90	182.0
86.90	666.0
87.80	655.0
90.80	102.0
91.90	589.0
93.00	955.0
94.00	2387.0
95.00	17224.0
96.00	1076.0
103.90	118.0
105.90	126.0
116.90	134.0
118.80	130.0
140.80	239.0
142.70	244.0
171.90	193.0
173.00	277.0
173.90	18488.0
174.90	1361.0
175.90	17680.0
176.90	1247.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
37.00	635.0
37.90	661.0
38.90	323.0
44.00	344.0
44.90	119.0
46.90	171.0
47.90	144.0
48.90	726.0
50.00	2797.0
51.00	832.0
56.00	265.0
56.90	513.0
60.00	148.0
60.90	777.0
61.90	852.0
63.00	670.0
64.00	116.0
67.90	1691.0
69.00	1499.0
69.90	144.0
71.90	133.0
72.90	794.0
73.90	2722.0
75.00	8050.0
76.00	620.0
77.00	120.0
78.90	656.0
79.80	204.0
80.90	791.0
81.90	177.0
86.90	564.0
87.80	528.0
91.90	568.0
93.00	865.0
94.00	2173.0
95.00	15837.0
96.00	984.0
103.90	115.0
105.90	105.0
116.80	128.0
118.80	138.0
140.80	247.0
142.80	233.0
171.90	180.0
172.90	309.0
173.90	17448.0
174.90	1289.0
175.90	16744.0
176.90	1105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72