


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092419\
 Data File : VV012957.D
 Acq On : 24 Sep 2019 12:52
 Operator : SY/MD
 Sample : BFB62
 Misc : 5.00G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB62

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
 Title : VOC Analysis
 Last Update : Wed Sep 25 08:42:02 2019

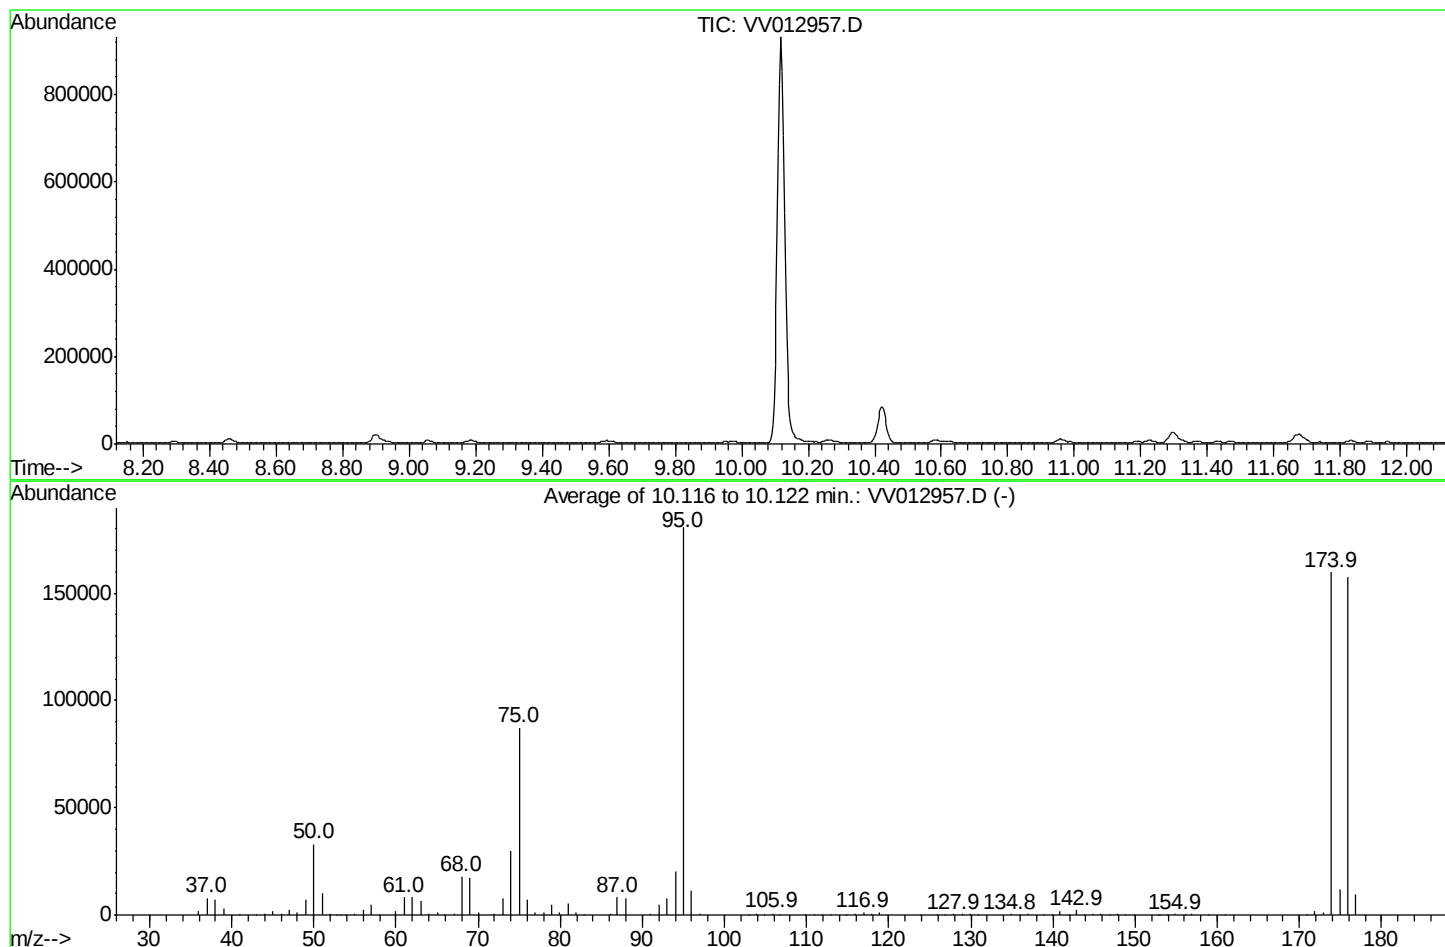

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	32938	PASS
75	95	30	80	48.3	87277	PASS
95	95	100	100	100.0	180757	PASS
96	95	5	9	6.4	11542	PASS
173	174	0.00	2	0.7	1045	PASS
174	95	50	120	88.4	159722	PASS
175	174	5	9	7.7	12222	PASS
176	174	95	101	98.6	157440	PASS
177	176	5	9	6.2	9813	PASS

Scan 2794 (10.074 min): VV012957.D
BFB62

m/z	Abundance
35.80	130.0
39.90	1446.0
44.00	1295.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
36.00	1721.0
37.00	8489.0
38.00	7600.0
39.10	3359.0
39.90	1351.0
40.90	135.0
43.00	132.0
44.00	1908.0
45.00	1794.0
46.00	314.0
47.00	2552.0
47.90	1163.0
49.00	7508.0
50.00	34344.0
51.00	10908.0
52.00	465.0
52.70	193.0
55.00	529.0
56.00	2491.0
57.00	4638.0
57.90	237.0
60.00	1678.0
61.00	8698.0
62.00	8888.0
63.00	6961.0
64.00	886.0
65.10	1368.0
65.80	169.0
67.00	484.0
68.00	18200.0
69.00	18256.0
70.00	1253.0
72.00	992.0
73.00	7520.0
74.00	30416.0
75.00	90088.0
76.00	7450.0
77.00	1181.0
78.00	1004.0
78.90	5274.0
79.90	1500.0
80.90	5436.0
81.90	1327.0
82.90	140.0
86.00	348.0
87.00	8051.0
88.00	7641.0
90.90	624.0
92.00	5123.0
93.00	8113.0
94.00	20976.0
95.00	184640.0
96.00	12104.0
97.00	416.0
102.90	119.0
103.90	705.0
104.80	248.0
105.90	890.0
106.70	208.0
109.90	117.0
110.90	146.0
111.80	103.0
112.80	125.0
114.80	242.0
115.90	589.0
116.90	1100.0
117.90	840.0
118.90	932.0
123.90	116.0
125.80	102.0
126.80	143.0
127.90	581.0
129.00	349.0
129.80	574.0
130.80	277.0
134.80	352.0
136.00	111.0
136.90	381.0
138.80	102.0
139.90	170.0
140.90	1891.0
141.90	303.0
142.90	2155.0
143.90	208.0
144.80	444.0
145.80	392.0
146.80	133.0
147.90	463.0
148.70	116.0
149.90	152.0
153.10	143.0
153.90	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

154.90	447.0
156.10	108.0
156.90	323.0
158.90	231.0
160.90	230.0
170.80	255.0
171.90	1540.0
173.90	160640.0
174.90	12486.0
175.90	157632.0
176.90	9816.0
177.90	320.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
36.00	1754.0
37.00	8239.0
38.00	7458.0
39.00	3395.0
40.00	1363.0
40.90	141.0
42.90	199.0
44.00	1960.0
45.00	1714.0
46.00	345.0
47.00	2628.0
48.00	1027.0
49.00	7309.0
50.00	34064.0
51.00	10806.0
52.00	382.0
52.80	171.0
53.10	174.0
53.80	110.0
55.00	490.0
56.00	2516.0
57.00	4751.0
57.90	236.0
60.00	1623.0
61.00	8511.0
62.00	8537.0
63.00	6663.0
63.90	942.0
65.10	1355.0
65.90	180.0
67.10	505.0
68.00	18456.0
69.00	18040.0
70.00	1174.0
72.00	895.0
73.00	7690.0
74.00	30880.0
75.00	90264.0
76.00	7096.0
76.90	1088.0
78.00	1009.0
78.90	5181.0
79.90	1446.0
80.90	5527.0
81.90	1297.0
82.90	175.0
86.10	334.0
86.90	8349.0
88.00	7871.0
90.90	605.0
92.00	5184.0
93.00	7918.0
94.00	20752.0
95.00	186688.0
96.00	11964.0
97.00	432.0
102.90	150.0
103.90	731.0
104.80	242.0
105.90	869.0
106.70	150.0
109.80	131.0
110.90	134.0
112.90	107.0
114.90	248.0
115.90	638.0
116.90	1214.0
117.90	741.0
118.80	975.0
123.90	121.0
125.80	131.0
126.70	122.0
127.90	607.0
128.90	331.0
129.90	536.0
130.80	335.0
134.90	325.0
136.00	134.0
137.00	376.0
138.70	110.0
139.80	165.0
140.90	1925.0
142.00	352.0
142.90	2416.0
143.80	132.0
144.90	418.0
145.80	392.0
146.90	155.0
147.90	435.0
148.70	105.0
149.90	121.0
152.80	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

153.10	127.0
153.80	124.0
154.90	475.0
156.10	117.0
156.90	345.0
159.00	201.0
160.90	222.0
170.90	220.0
171.80	1557.0
173.00	1600.0
173.90	164928.0
174.90	12677.0
175.90	162624.0
176.90	10127.0
177.90	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

m/z	Abundance
36.00	1639.0
37.00	7119.0
38.00	6591.0
39.10	2983.0
40.00	1384.0
41.00	113.0
43.00	250.0
44.00	1981.0
45.00	1438.0
46.00	315.0
47.00	2422.0
48.00	893.0
49.00	6301.0
50.00	30408.0
51.00	9506.0
52.00	352.0
53.20	203.0
53.80	110.0
55.00	448.0
56.00	2399.0
57.00	4575.0
57.90	212.0
60.00	1410.0
61.00	7611.0
62.00	7286.0
63.00	5837.0
63.90	921.0
65.00	1146.0
65.80	163.0
67.10	485.0
68.00	16688.0
69.00	16127.0
70.00	1051.0
71.90	842.0
73.00	7246.0
74.00	28296.0
75.00	81480.0
76.00	6406.0
76.90	893.0
78.00	919.0
78.90	4459.0
79.90	1248.0
80.90	4868.0
81.90	1135.0
82.90	158.0
86.10	288.0
86.90	7859.0
88.00	7425.0
90.90	579.0
92.00	4619.0
93.00	7006.0
94.00	18672.0
95.00	170944.0
96.00	10558.0
97.00	310.0
102.90	174.0
103.90	719.0
104.80	211.0
105.90	798.0
106.80	130.0
109.80	115.0
110.80	118.0
112.90	127.0
114.90	204.0
116.00	624.0
116.90	1202.0
117.80	588.0
118.80	906.0
123.90	123.0
125.80	101.0
127.90	602.0
128.90	312.0
129.90	477.0
130.80	335.0
134.90	292.0
136.00	119.0
137.00	324.0
138.70	105.0
139.80	166.0
140.90	1707.0
142.00	298.0
142.90	2277.0
144.90	406.0
145.80	300.0
147.00	156.0
147.80	366.0
148.70	117.0
152.80	107.0
153.00	106.0
154.90	504.0
155.90	105.0
156.80	305.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62

159.00	187.0
160.90	208.0
171.00	164.0
171.90	1480.0
173.00	1535.0
173.90	153600.0
174.90	11503.0
175.90	152064.0
176.90	9498.0
177.90	229.0

Instrument :
MSVOA_V
ClientSampleId :
BFB62