

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092420\
 Data File : VV018421.D
 Acq On : 24 Sep 2020 12:13
 Operator : SY/MD
 Sample : L4110-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL4

Quant Time: Sep 25 05:02:41 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 25 04:36:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	272961	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	270323	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	134707	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	92444	41.56	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.12%
7) Chloroethane-d5	1.58	69	83524	45.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.78%
11) 1,1-Dichloroethene-d2	2.12	63	144894	35.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.02%
21) 2-Butanone-d5	3.92	46	154677	113.60	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	113.60%
24) Chloroform-d	4.38	84	198148	51.34	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.68%
26) 1,2-Dichloroethane-d4	5.06	65	133219	53.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.70%
32) Benzene-d6	5.08	84	401514	51.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.76%
36) 1,2-Dichloropropane-d6	6.09	67	130043	52.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.78%
41) Toluene-d8	7.34	98	361859	51.31	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.62%
43) trans-1,3-Dichloropropene-	7.64	79	64756	51.83	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	103.66%
47) 2-Hexanone-d5	8.11	63	95966	103.04	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.04%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	151724	49.16	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.32%
64) 1,2-Dichlorobenzene-d4	11.65	152	160180	57.90	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	115.80%


Target Compounds					Ovalue
13) Acetone	2.20	43	10245	9.397 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092420\
Data File : VV018421.D
Acq On : 24 Sep 2020 12:13
Operator : SY/MD
Sample : L4110-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AL4

Quant Time: Sep 25 05:02:41 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 25 04:36:20 2020
Response via : Initial Calibration

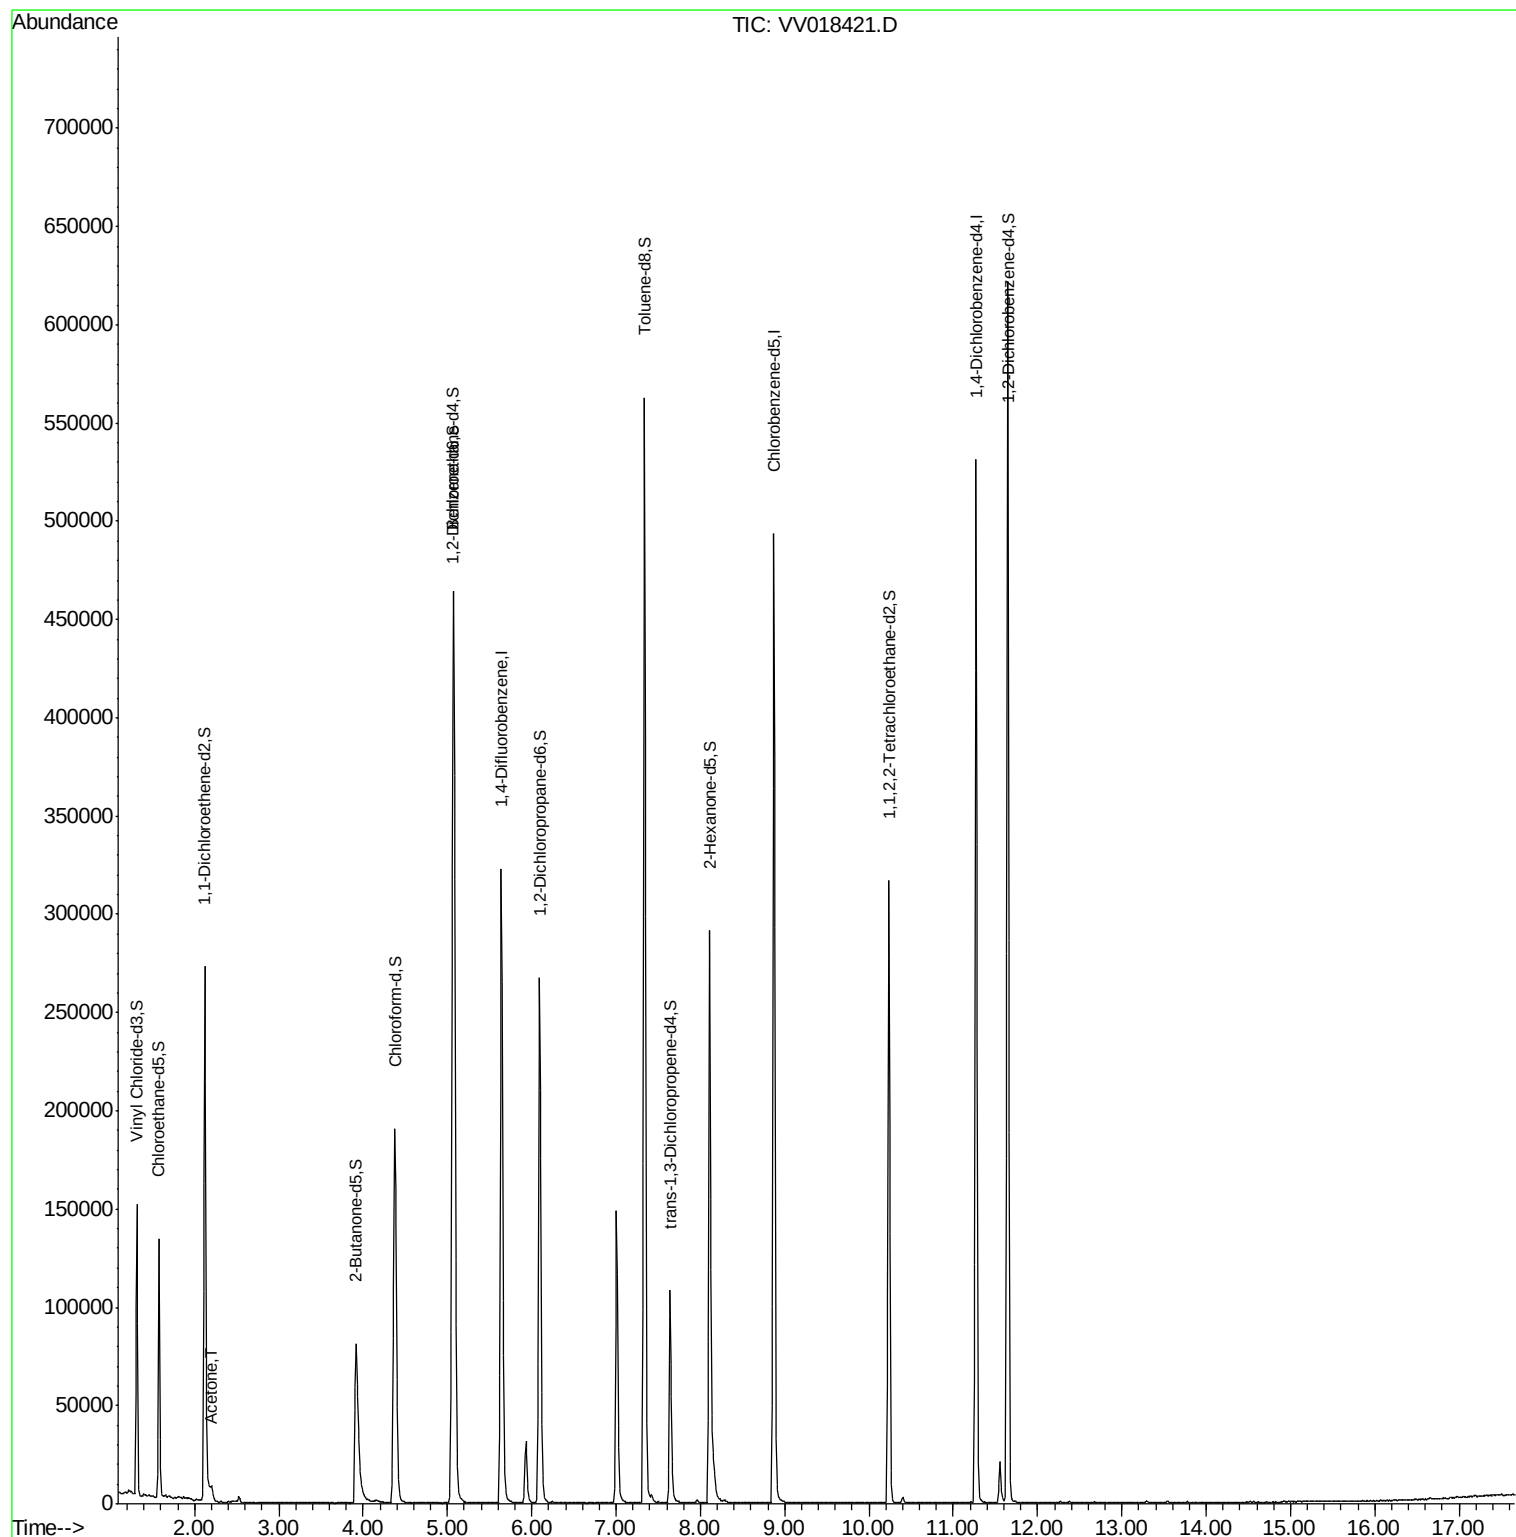

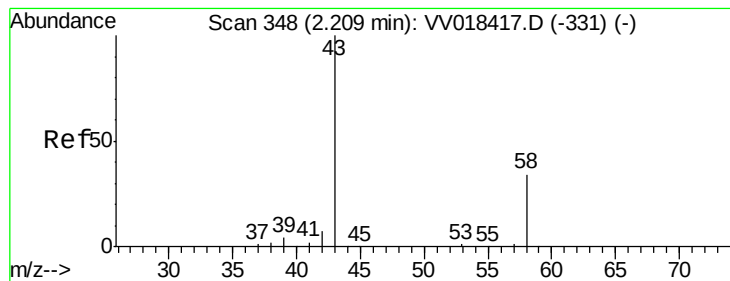

#13
 Acetone
 Concen: 9.397 ug/L
 RT: 2.20 min Scan# 345
 Delta R.T. -0.01 min
 Lab File: VV018421.D
 Acq: 24 Sep 2020 12:13

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AL4

Tot Ion: 43 Resp: 10245
 Ion Ratio Lower Upper
 43 100
 58 34.0 0.0 67.4

