

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092420\
 Data File : VV018424.D
 Acq On : 24 Sep 2020 13:21
 Operator : SY/MD
 Sample : L4110-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK5

Quant Time: Sep 25 05:18:10 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 25 04:36:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	303614	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	296243	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	147448	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	112012	45.27	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.54%
7) Chloroethane-d5	1.58	69	88074	43.50	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.00%
11) 1,1-Dichloroethene-d2	2.12	63	153713	33.87	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.74%
21) 2-Butanone-d5	3.91	46	122851	81.12	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	81.12%
24) Chloroform-d	4.38	84	180176	41.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.94%
26) 1,2-Dichloroethane-d4	5.06	65	120538	43.80	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.60%
32) Benzene-d6	5.08	84	375811	44.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.62%
36) 1,2-Dichloropropane-d6	6.09	67	117536	43.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.24%
41) Toluene-d8	7.34	98	338363	43.78	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.56%
43) trans-1,3-Dichloropropene-	7.64	79	58083	42.42	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.84%
47) 2-Hexanone-d5	8.11	63	72680	71.21	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	71.21%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	127992	37.84	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	75.68%
64) 1,2-Dichlorobenzene-d4	11.65	152	139551	46.08	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.16%


Target Compounds					Ovalue
13) Acetone	2.20	43	10617	8.755 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092420\
Data File : VV018424.D
Acq On : 24 Sep 2020 13:21
Operator : SY/MD
Sample : L4110-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AK5

Quant Time: Sep 25 05:18:10 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 25 04:36:20 2020
Response via : Initial Calibration

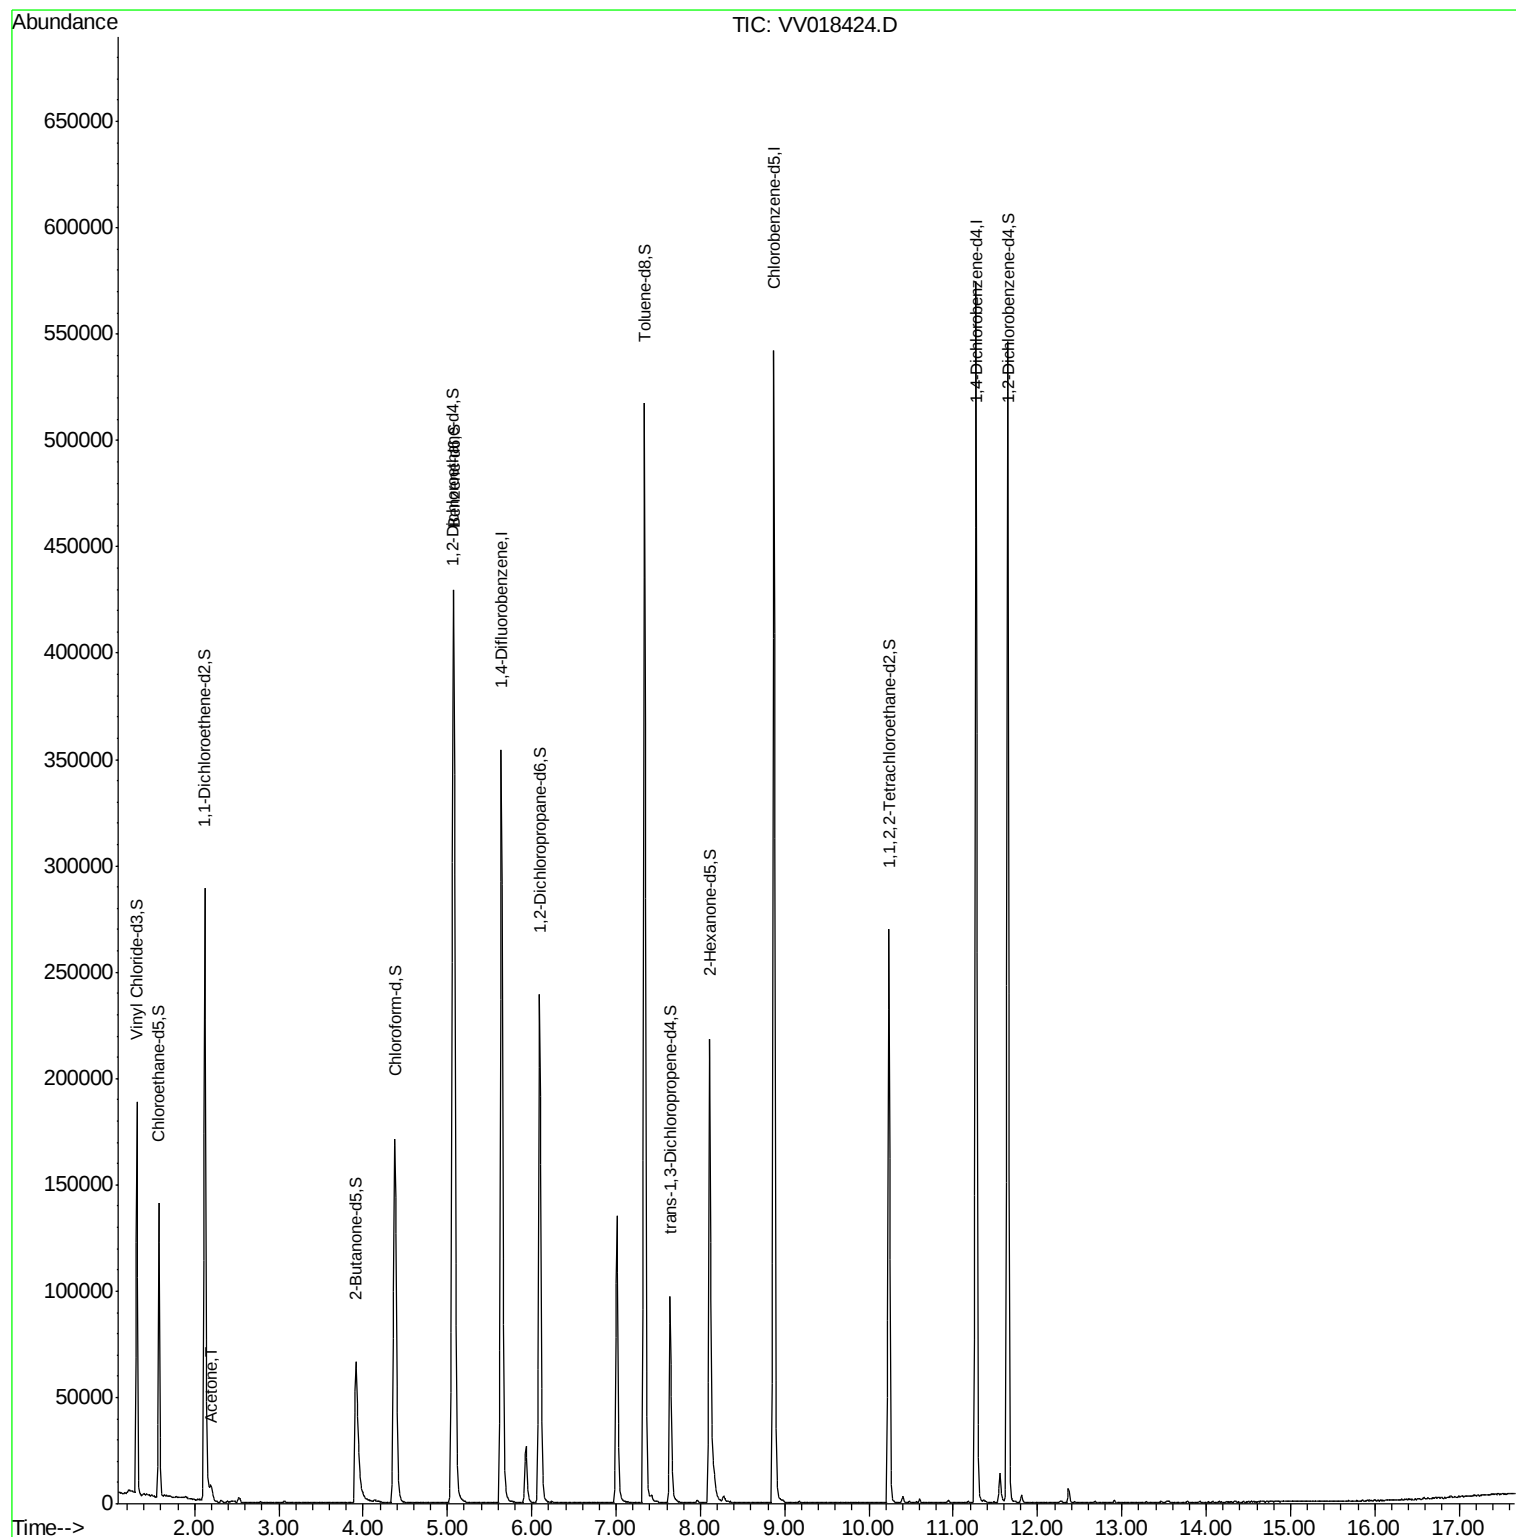

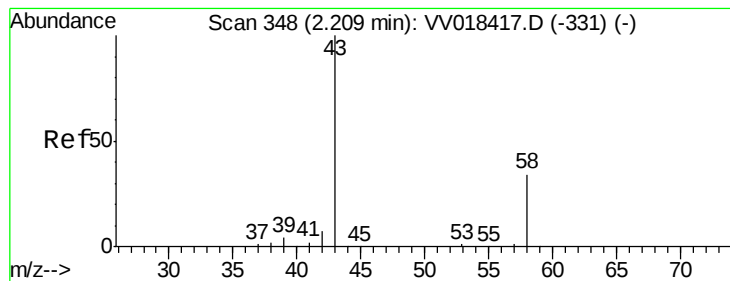

#13
 Acetone
 Concen: 8.755 ug/L
 RT: 2.20 min Scan# 344
 Delta R.T. -0.01 min
 Lab File: VV018424.D
 Acq: 24 Sep 2020 13:21

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AK5

Tot Ion: 43 Resp: 10617
 Ion Ratio Lower Upper
 43 100
 58 31.3 0.0 67.4

