


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092420\
 Data File : VV018416.D
 Acq On : 24 Sep 2020 08:22
 Operator : SY/MD
 Sample : BFB98
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB98

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis
 Last Update : Mon Sep 28 03:12:36 2020

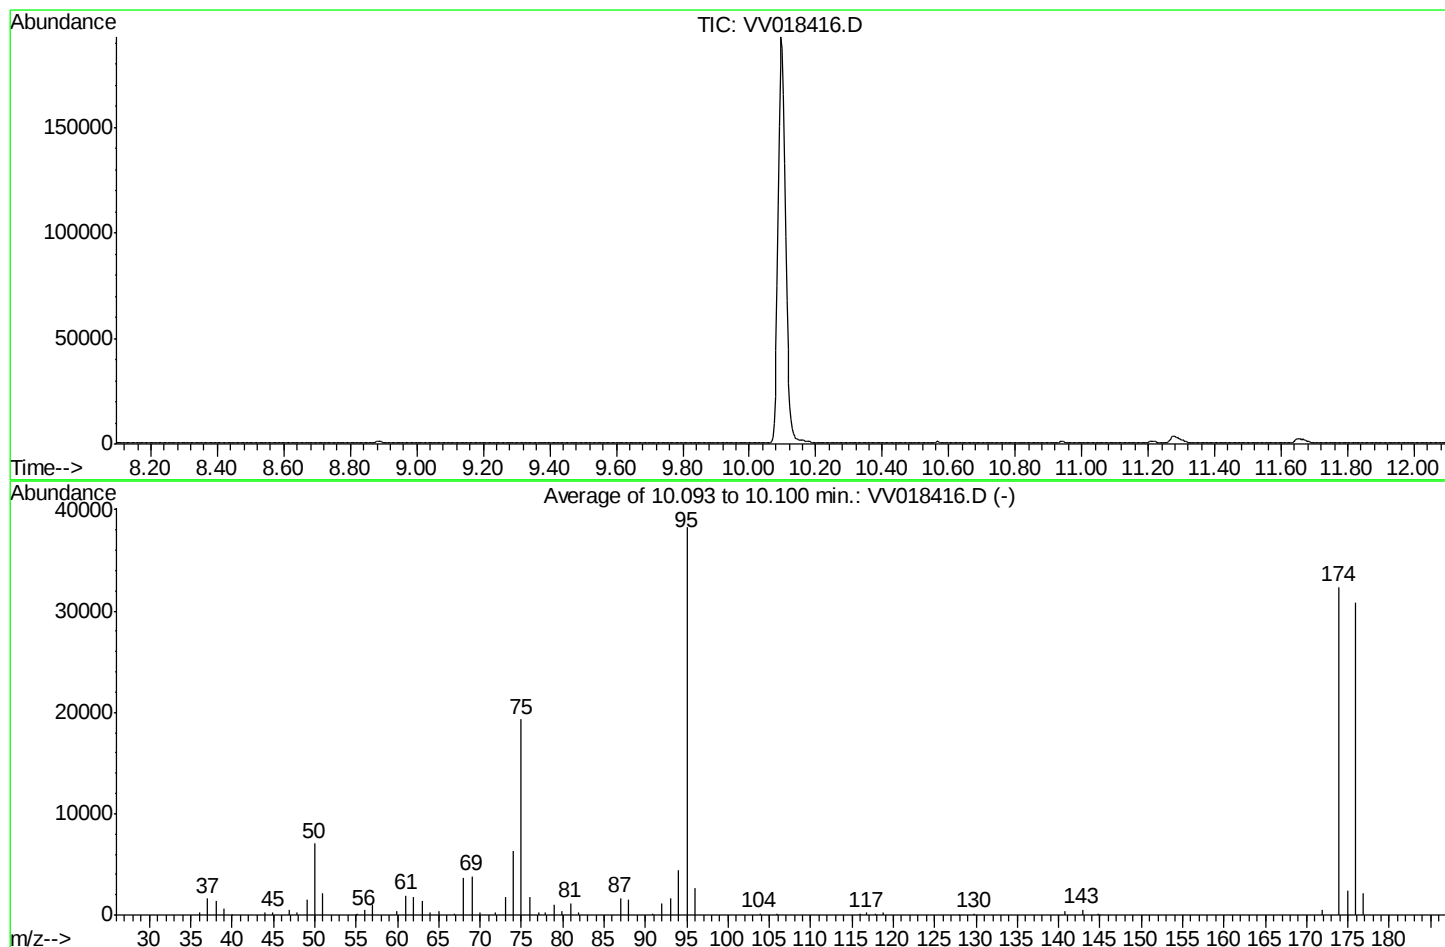

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	7044	PASS
75	95	30	80	50.4	19288	PASS
95	95	100	100	100.0	38269	PASS
96	95	5	9	6.8	2597	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.6	32368	PASS
175	174	5	9	7.5	2442	PASS
176	174	95	101	95.1	30786	PASS
177	176	5	9	6.8	2095	PASS

Scan 2790 (10.061 min): VV018416.D
BFB98

m/z	Abundance
39.90	227.0
43.90	253.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
36.00	318.0
37.00	1559.0
38.00	1344.0
39.00	649.0
39.90	270.0
43.90	480.0
44.90	269.0
46.90	458.0
47.80	250.0
49.00	1445.0
50.00	6872.0
51.00	2181.0
54.90	123.0
56.00	472.0
57.00	971.0
59.90	382.0
61.00	1949.0
62.00	1710.0
63.00	1389.0
64.00	203.0
65.00	358.0
66.90	152.0
68.00	3611.0
69.00	3797.0
70.00	342.0
71.90	186.0
73.00	1718.0
74.00	6290.0
75.00	18536.0
76.00	1689.0
77.10	202.0
77.80	203.0
78.90	1029.0
79.90	420.0
80.90	1156.0
81.90	264.0
87.00	1688.0
87.90	1472.0
90.90	136.0
91.90	1156.0
93.00	1551.0
94.00	4323.0
95.00	36776.0
96.00	2537.0
103.90	140.0
105.90	137.0
115.90	158.0
116.80	246.0
117.80	163.0
118.80	229.0
129.80	172.0
140.80	285.0
142.90	515.0
144.80	152.0
171.90	424.0
173.90	30288.0
174.90	2422.0
175.90	29240.0
176.90	1979.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
36.00	312.0
37.00	1663.0
38.00	1438.0
38.90	661.0
39.90	270.0
43.90	485.0
45.00	326.0
46.90	464.0
47.90	294.0
49.00	1522.0
50.00	7279.0
51.00	2270.0
55.10	124.0
56.00	524.0
57.00	999.0
59.90	363.0
61.00	2020.0
62.00	1813.0
63.00	1459.0
64.00	227.0
65.00	353.0
67.00	129.0
68.00	3796.0
69.00	3991.0
70.00	317.0
71.90	207.0
73.00	1830.0
74.00	6557.0
75.00	19944.0
76.00	1795.0
77.00	251.0
77.90	213.0
79.00	1086.0
79.90	432.0
80.90	1222.0
81.90	304.0
87.00	1708.0
87.90	1580.0
90.90	141.0
92.00	1221.0
93.00	1704.0
94.00	4523.0
95.00	39616.0
96.00	2718.0
103.80	144.0
105.90	131.0
115.90	164.0
116.80	249.0
117.90	169.0
118.80	229.0
129.80	178.0
140.80	331.0
142.90	553.0
144.80	174.0
171.90	466.0
173.90	33480.0
174.90	2510.0
175.90	31800.0
176.90	2162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98

m/z	Abundance
36.00	309.0
37.00	1649.0
38.00	1445.0
39.00	644.0
39.90	238.0
44.00	455.0
45.00	356.0
47.00	427.0
47.90	307.0
49.00	1432.0
50.00	6981.0
51.00	2165.0
55.00	114.0
56.00	514.0
57.00	922.0
59.90	340.0
61.00	1854.0
62.00	1741.0
63.00	1390.0
63.90	228.0
65.00	324.0
67.00	107.0
68.00	3651.0
69.00	3759.0
70.00	273.0
71.90	199.0
73.00	1783.0
74.00	6164.0
75.00	19384.0
76.00	1781.0
77.00	270.0
77.90	188.0
78.90	1065.0
79.90	390.0
80.90	1186.0
81.80	286.0
86.90	1563.0
87.90	1600.0
90.90	137.0
92.00	1179.0
93.00	1654.0
94.00	4352.0
95.00	38416.0
96.00	2537.0
103.80	154.0
105.90	132.0
115.90	129.0
116.80	231.0
118.00	149.0
118.80	196.0
127.90	106.0
129.80	151.0
140.80	353.0
142.90	533.0
145.00	176.0
171.90	457.0
173.90	33336.0
174.90	2396.0
175.90	31320.0
176.90	2145.0

Instrument :
MSVOA_V
ClientSampleId :
BFB98