

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
 Data File : VV022316.D
 Acq On : 24 Sep 2021 12:36
 Operator : SY/MD
 Sample : M3814-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6X9

Quant Time: Sep 25 04:31:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 25 04:30:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	125626	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	124639	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	54948	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	28307	4.472	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	89.400%	
7) Chloroethane-d5	1.564	69	33734	4.554	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	91.000%	
11) 1,1-Dichloroethene-d2	2.104	63	49386	3.272	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	65.400%	
20) 2-Butanone-d5	3.879	46	102285	39.541	ug/L	-0.03
Spiked Amount	50.000	Range 40 - 130	Recovery	=	79.080%	
24) Chloroform-d	4.352	84	81629	4.496	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	90.000%	
26) 1,2-Dichloroethane-d4	5.037	65	39926	4.603	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.000%	
32) Benzene-d6	5.053	84	161833	4.617	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.400%	
36) 1,2-Dichloropropane-d6	6.072	67	53086	4.850	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	97.000%	
41) Toluene-d8	7.320	98	132886	4.199	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.000%	
43) trans-1,3-Dichloroprop...	7.628	79	12817	3.834	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	76.600%	
46) 2-Hexanone-d5	8.091	63	80517	38.738	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	77.480%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	35594	3.863	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	77.200%	
66) 1,2-Dichlorobenzene-d4	11.628	152	49572	4.807	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.200%	
Target Compounds					Qvalue	
13) Acetone	2.166	43	6833	4.659	ug/L	98
42) Toluene	7.400	91	4290	0.124	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022316.D
Acq On : 24 Sep 2021 12:36
Operator : SY/MD
Sample : M3814-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6X9

Quant Time: Sep 25 04:31:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 25 04:30:06 2021
Response via : Initial Calibration




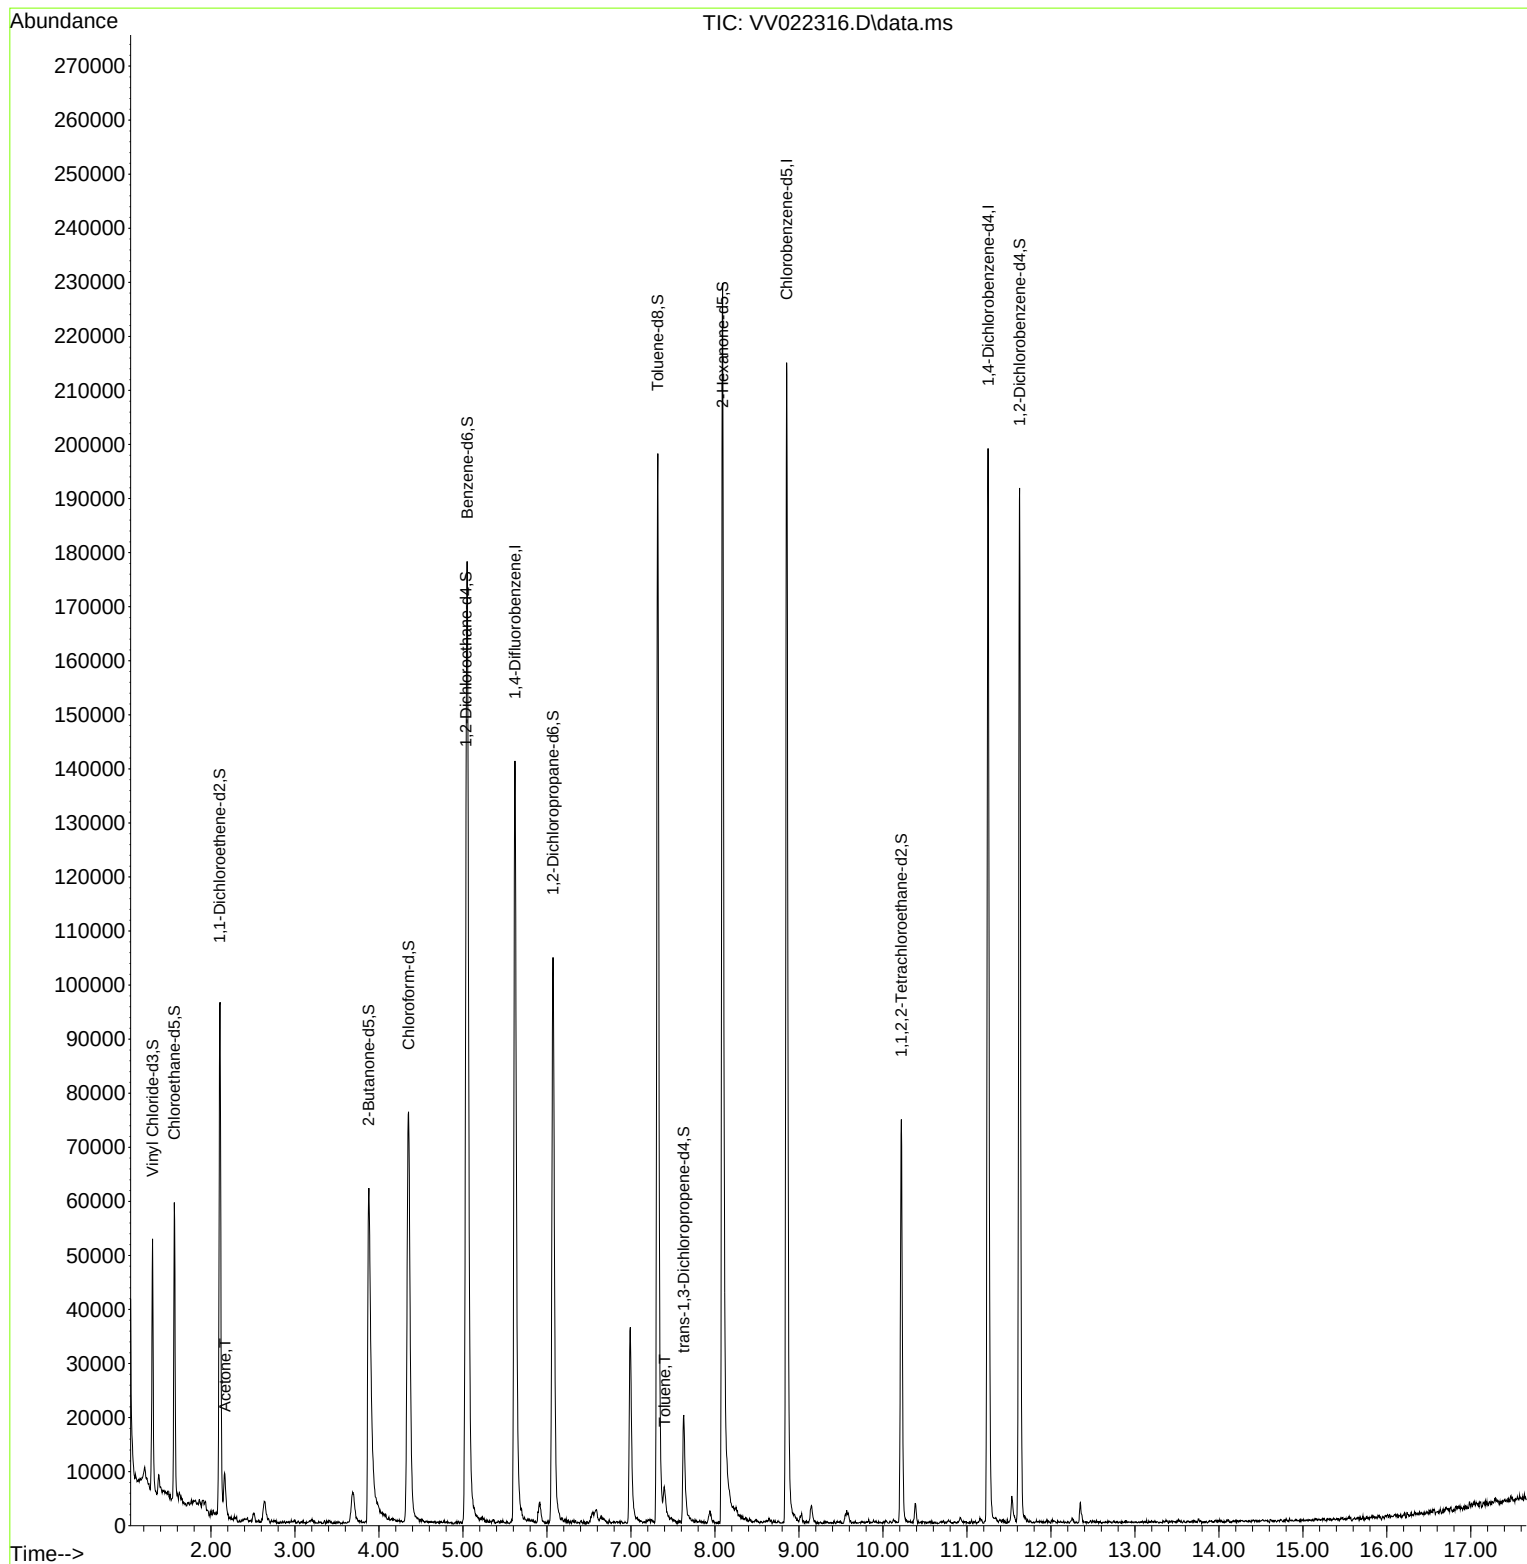


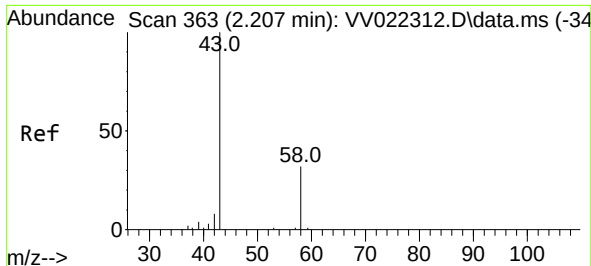

#13
Acetone
Concen: 4.659 ug/L
RT: 2.166 min Scan# 350
Delta R.T. -0.042 min
Lab File: VV022316.D
Acq: 24 Sep 2021 12:36

Instrument :
MSVOA_V
ClientSampled :
GB6X9

Tgt Ion: 43 Resp: 6833
Ion Ratio Lower Upper
43 100
58 34.4 0.0 66.2

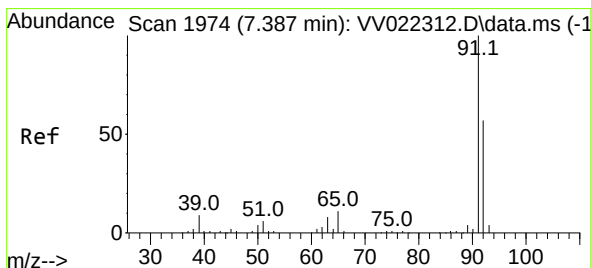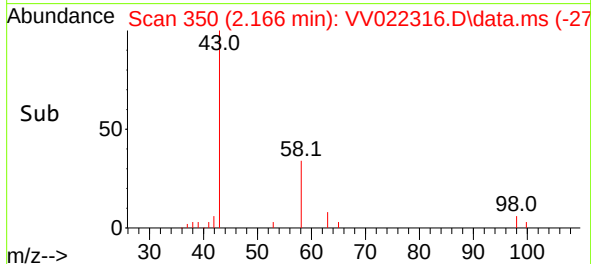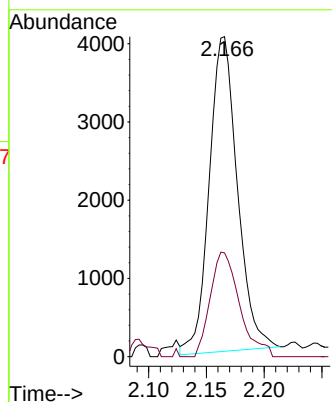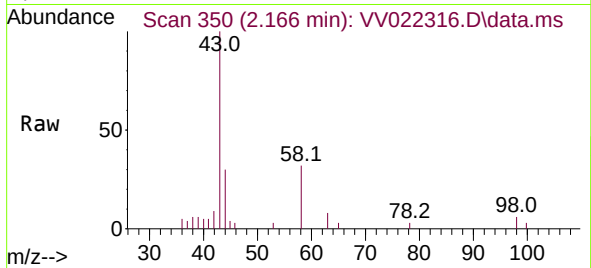

#42
Toluene
Concen: 0.124 ug/L
RT: 7.400 min Scan# 1978
Delta R.T. 0.013 min
Lab File: VV022316.D
Acq: 24 Sep 2021 12:36

Tgt Ion: 91 Resp: 4290
Ion Ratio Lower Upper
91 100
92 69.0 40.6 75.4

