

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
 Data File : VV022317.D
 Acq On : 24 Sep 2021 13:00
 Operator : SY/MD
 Sample : M3814-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6Y0

Quant Time: Sep 25 04:31:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 25 04:30:06 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	130258	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	128222	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	57528	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	26856	4.092	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.800%
7) Chloroethane-d5	1.564	69	33339	4.340	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.800%
11) 1,1-Dichloroethene-d2	2.105	63	49815	3.183	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.600%
20) 2-Butanone-d5	3.905	46	111254	41.479	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	82.960%
24) Chloroform-d	4.352	84	82464	4.380	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
26) 1,2-Dichloroethane-d4	5.040	65	39692	4.413	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.200%
32) Benzene-d6	5.053	84	161502	4.479	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.600%
36) 1,2-Dichloropropane-d6	6.072	67	54019	4.798	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.000%
41) Toluene-d8	7.320	98	131739	4.046	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.000%
43) trans-1,3-Dichloroprop...	7.628	79	13488	3.922	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.400%
46) 2-Hexanone-d5	8.091	63	82911	38.775	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.560%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	35616	3.757	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	75.200%
66) 1,2-Dichlorobenzene-d4	11.628	152	50429	4.671	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.400%
Target Compounds					Qvalue	
13) Acetone	2.201	43	21373	14.054	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022317.D
Acq On : 24 Sep 2021 13:00
Operator : SY/MD
Sample : M3814-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6Y0

Quant Time: Sep 25 04:31:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 25 04:30:06 2021
Response via : Initial Calibration

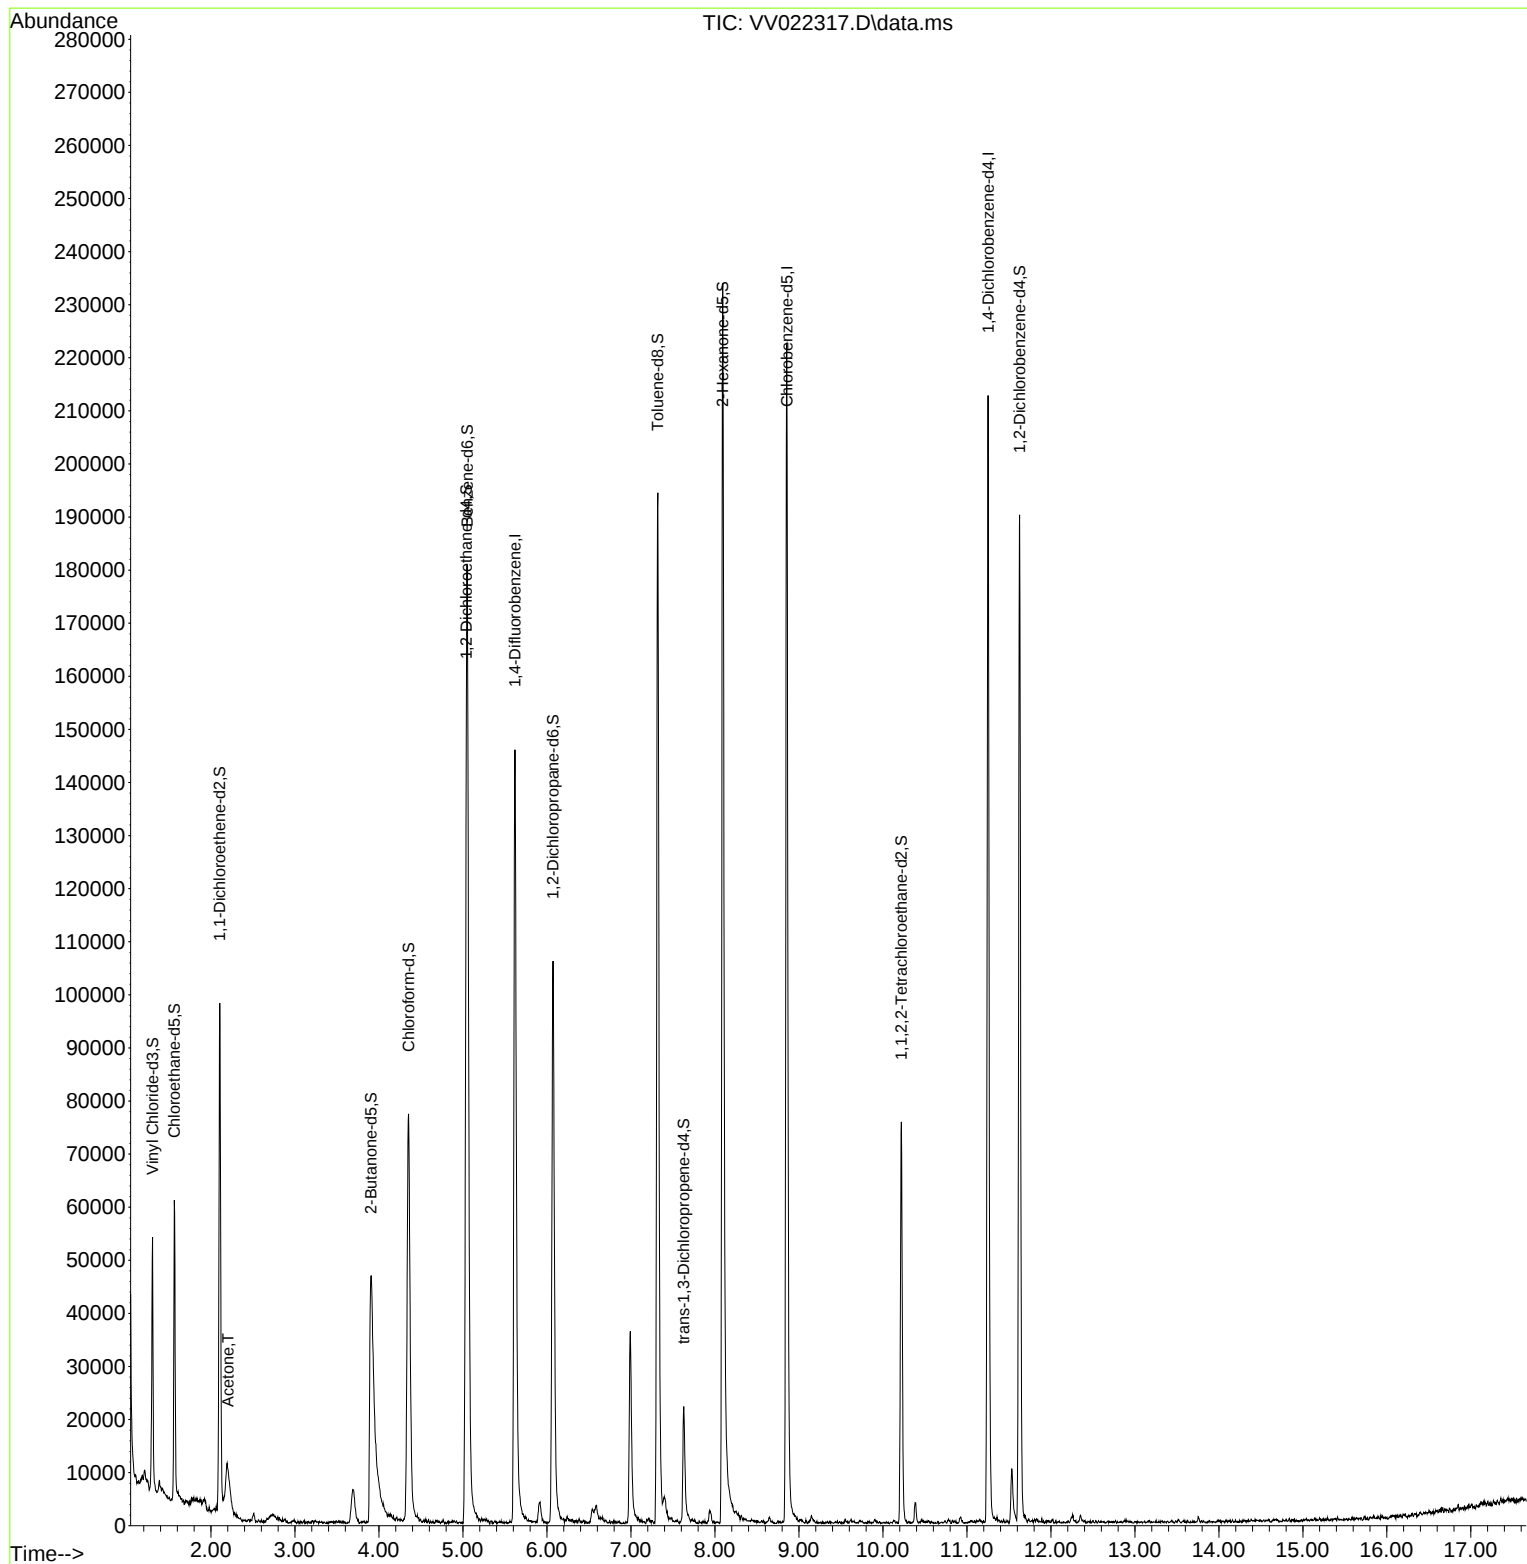

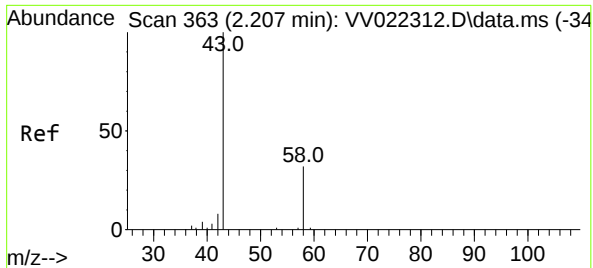

#13
 Acetone
 Concen: 14.054 ug/L
 RT: 2.201 min Scan# 361
 Delta R.T. -0.006 min
 Lab File: VV022317.D
 Acq: 24 Sep 2021 13:00

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6Y0

Tgt Ion:	43	Resp:	21373
Ion	Ratio	Lower	Upper
43	100		
58	35.0	0.0	66.2

