

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
 Data File : VV022314.D
 Acq On : 24 Sep 2021 11:49
 Operator : SY/MD
 Sample : M3878-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2J7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	94	rVB	46756	50127	11.14%	1.381%
2	1.564	156	163	171	rBV	56584	64673	14.37%	1.782%
3	2.101	319	330	342	rBV	97232	141584	31.46%	3.901%
4	2.503	444	455	470	rBV2	10092	18716	4.16%	0.516%
5	3.912	881	893	944	rBV2	33494	187523	41.67%	5.166%
6	4.346	1011	1028	1063	rBV	75407	196793	43.73%	5.422%
7	5.043	1228	1245	1279	rBV3	178611	450039	100.00%	12.399%
8	5.227	1289	1302	1315	rVB3	5048	12056	2.68%	0.332%
9	5.616	1411	1423	1453	rBV	137978	292563	65.01%	8.060%
10	5.905	1504	1513	1527	rVB8	3940	8809	1.96%	0.243%
11	6.069	1551	1564	1589	rBV	104256	218706	48.60%	6.026%
12	6.989	1836	1850	1866	rBV2	34746	68017	15.11%	1.874%
13	7.317	1940	1952	1971	rBV	194391	345228	76.71%	9.511%
14	7.625	2039	2048	2075	rBV2	20254	40330	8.96%	1.111%
15	7.860	2114	2121	2134	rVB9	2787	5326	1.18%	0.147%
16	8.091	2182	2193	2219	rBV	222959	439266	97.61%	12.102%
17	8.853	2419	2430	2454	rBV	218844	360681	80.14%	9.937%
18	10.217	2843	2854	2873	rBV	74370	117368	26.08%	3.234%
19	11.249	3164	3175	3198	rBV	197344	316775	70.39%	8.727%
20	11.625	3281	3292	3311	rBV	182105	295089	65.57%	8.130%




Sum of corrected areas: 3629669

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022314.D
Acq On : 24 Sep 2021 11:49
Operator : SY/MD
Sample : M3878-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

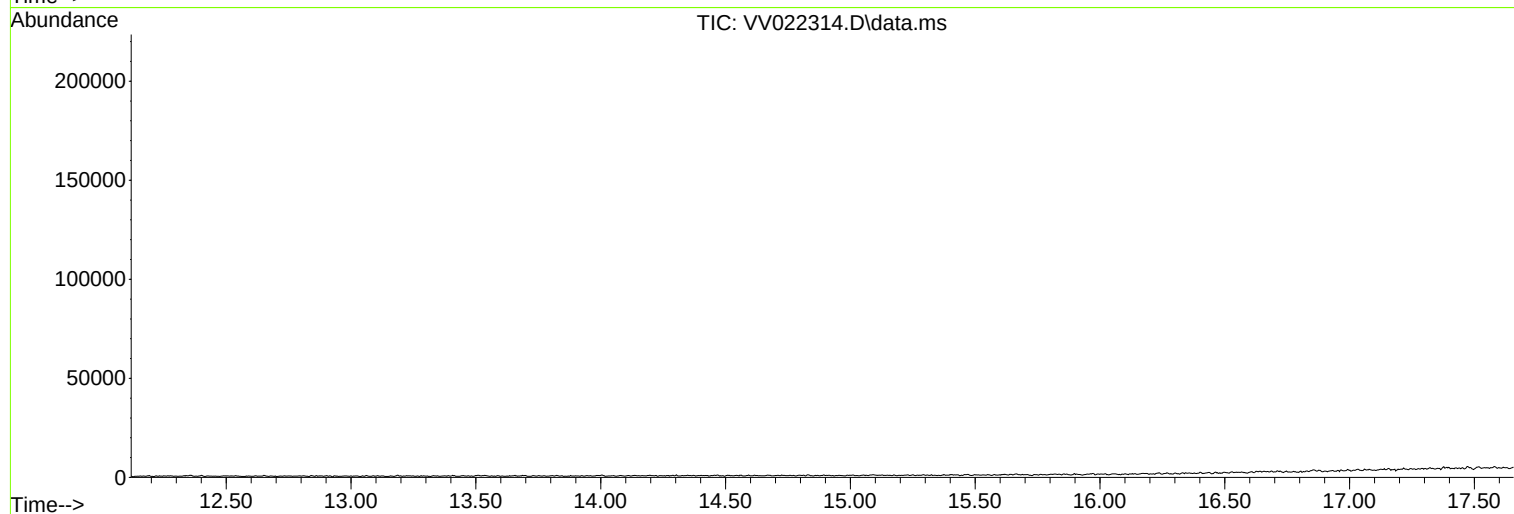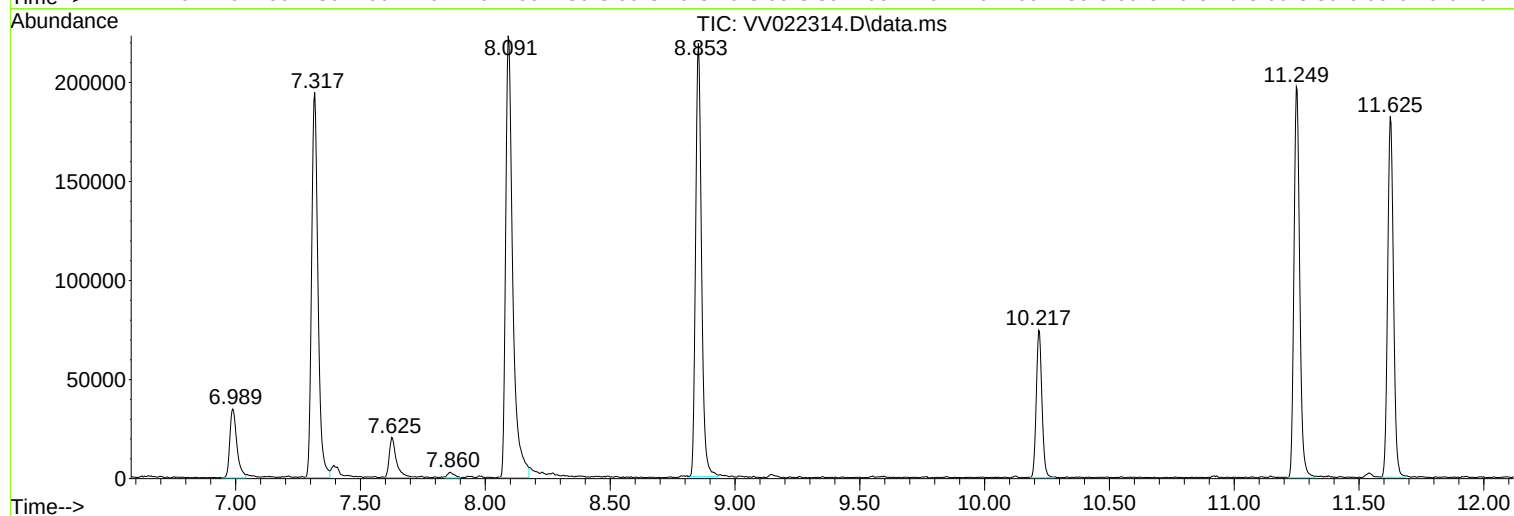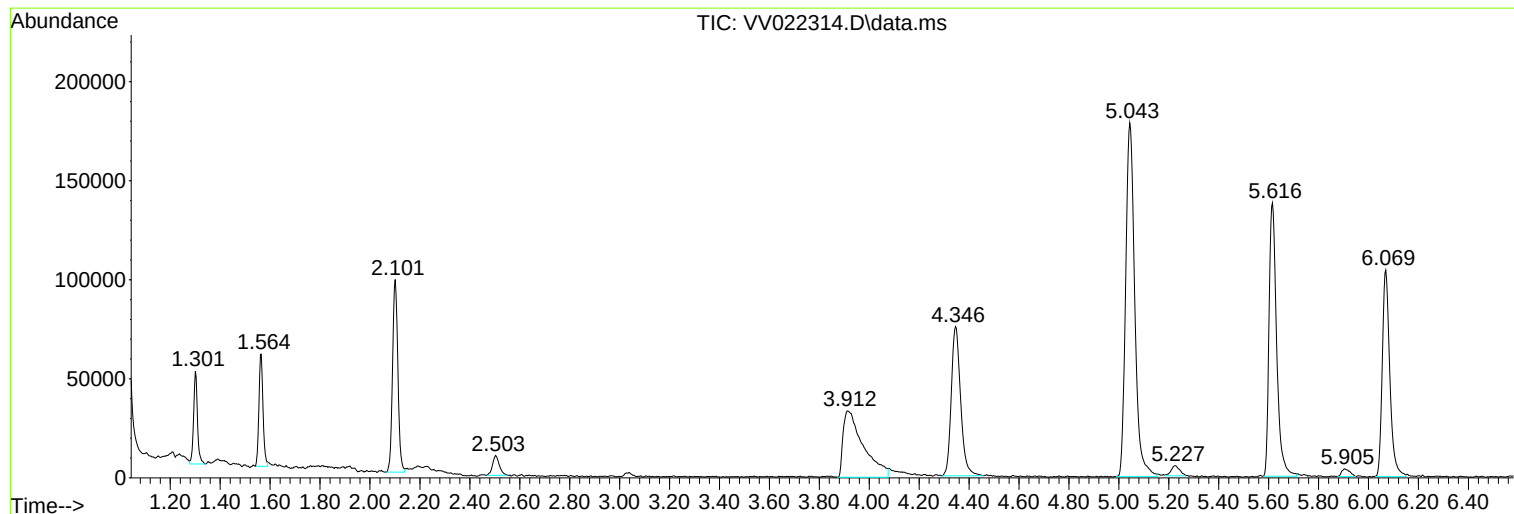

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022314.D
Acq On : 24 Sep 2021 11:49
Operator : SY/MD
Sample : M3878-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022314.D
Acq On : 24 Sep 2021 11:49
Operator : SY/MD
Sample : M3878-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2J7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
