

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
 Data File : VV022315.D
 Acq On : 24 Sep 2021 12:12
 Operator : SY/MD
 Sample : M3878-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW2N8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	93	rVB	49649	50170	10.54%	1.348%
2	1.564	155	163	177	rBV	54822	64940	13.64%	1.745%
3	2.101	319	330	341	rBV	100715	143880	30.22%	3.866%
4	2.503	448	455	464	rBV6	3410	5898	1.24%	0.158%
5	3.915	882	894	931	rBV2	40194	184853	38.83%	4.967%
6	4.349	1013	1029	1068	rBV2	79738	202862	42.61%	5.451%
7	5.050	1229	1247	1281	rBV2	189255	476118	100.00%	12.794%
8	5.227	1291	1302	1315	rVB3	4348	9654	2.03%	0.259%
9	5.619	1412	1424	1455	rBV	136647	290081	60.93%	7.795%
10	5.911	1505	1515	1532	rVB6	4767	11592	2.43%	0.311%
11	6.072	1552	1565	1591	rBV	108722	230559	48.42%	6.195%
12	6.992	1841	1851	1872	rBV	36743	71966	15.12%	1.934%
13	7.320	1942	1953	1971	rBV	199160	364760	76.61%	9.801%
14	7.400	1974	1978	1994	rVB3	5974	10825	2.27%	0.291%
15	7.628	2040	2049	2060	rBV2	22467	39199	8.23%	1.053%
16	7.863	2113	2122	2130	rBV6	2895	4819	1.01%	0.129%
17	8.095	2183	2194	2223	rBV	245005	470697	98.86%	12.648%
18	8.857	2420	2431	2453	rBV	207562	350434	73.60%	9.417%
19	10.220	2844	2855	2868	rBV	76431	122131	25.65%	3.282%
20	11.252	3165	3176	3195	rBV	192936	302079	63.45%	8.117%
21	11.628	3281	3293	3312	rBV	195179	313969	65.94%	8.437%




Sum of corrected areas: 3721486

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022315.D
Acq On : 24 Sep 2021 12:12
Operator : SY/MD
Sample : M3878-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2N8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

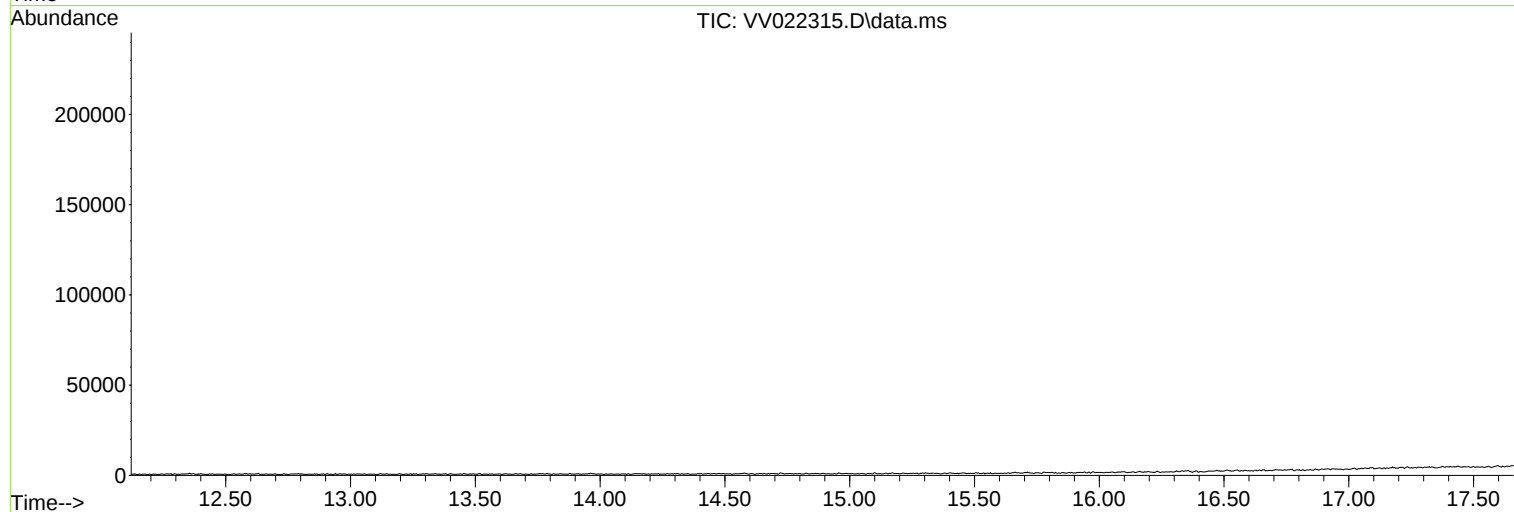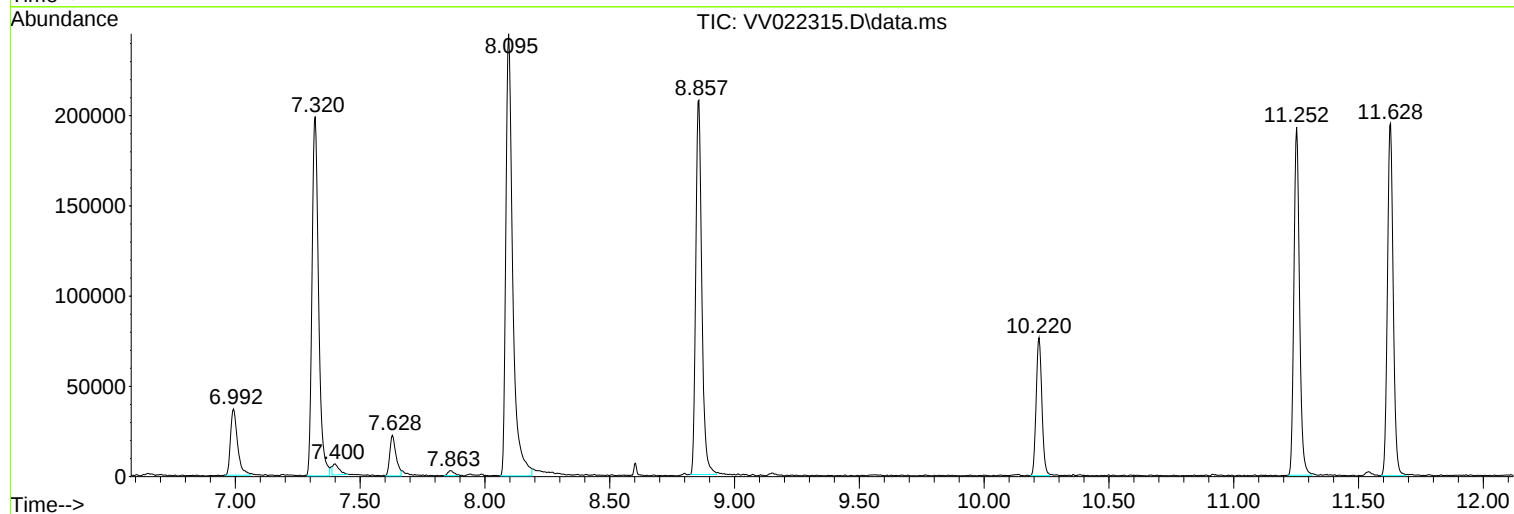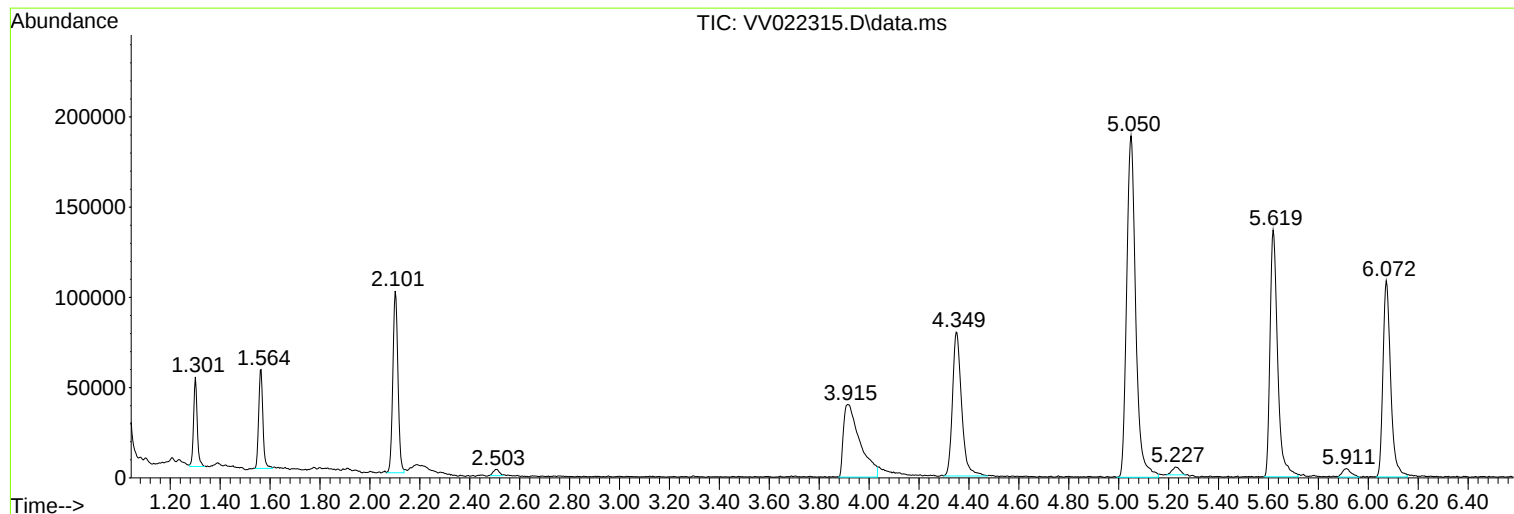

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022315.D
Acq On : 24 Sep 2021 12:12
Operator : SY/MD
Sample : M3878-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2N8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022315.D
Acq On : 24 Sep 2021 12:12
Operator : SY/MD
Sample : M3878-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW2N8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
