

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
 Data File : VV022316.D
 Acq On : 24 Sep 2021 12:36
 Operator : SY/MD
 Sample : M3814-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6X9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	93	rVB	46673	52540	11.71%	1.435%
2	1.564	156	163	173	rBV	54661	62099	13.84%	1.696%
3	2.108	322	332	343	rBV	94630	140305	31.27%	3.833%
4	2.162	343	349	361	rVB	7757	13096	2.92%	0.358%
5	2.635	484	496	509	rBV4	3863	9292	2.07%	0.254%
6	3.686	809	823	836	rBV6	5562	15429	3.44%	0.422%
7	3.879	874	883	914	rBV	61754	172004	38.34%	4.699%
8	4.352	1013	1030	1055	rBV2	75820	194539	43.36%	5.315%
9	5.050	1229	1247	1273	rBV3	177942	448641	100.00%	12.256%
10	5.619	1413	1424	1446	rBV	140489	287274	64.03%	7.848%
11	5.911	1510	1515	1526	rVB6	3429	6034	1.34%	0.165%
12	6.072	1550	1565	1592	rBV	104696	221824	49.44%	6.060%
13	6.587	1716	1725	1736	rVB7	2069	4612	1.03%	0.126%
14	6.992	1839	1851	1872	rBV2	36286	70793	15.78%	1.934%
15	7.320	1941	1953	1971	rBV	197845	350308	78.08%	9.570%
16	7.397	1972	1977	1992	rVB7	5696	11314	2.52%	0.309%
17	7.628	2040	2049	2066	rBV2	20049	39459	8.80%	1.078%
18	7.940	2135	2146	2155	rBV4	2311	4490	1.00%	0.123%
19	8.091	2183	2193	2229	rBV	229369	431924	96.27%	11.800%
20	8.853	2419	2430	2452	rBV	214599	361662	80.61%	9.880%
21	9.149	2512	2522	2532	rBV6	3235	6269	1.40%	0.171%
22	10.220	2842	2855	2870	rBV	74559	117008	26.08%	3.197%
23	10.387	2898	2907	2915	rVB4	3689	5694	1.27%	0.156%
24	11.252	3166	3176	3198	rBV	198444	317957	70.87%	8.686%
25	11.535	3253	3264	3279	rBV6	4917	8486	1.89%	0.232%
26	11.628	3279	3293	3308	rBV	191181	301627	67.23%	8.240%
27	12.352	3506	3518	3527	rBV6	3876	5802	1.29%	0.159%




Sum of corrected areas: 3660482

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022316.D
Acq On : 24 Sep 2021 12:36
Operator : SY/MD
Sample : M3814-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6X9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

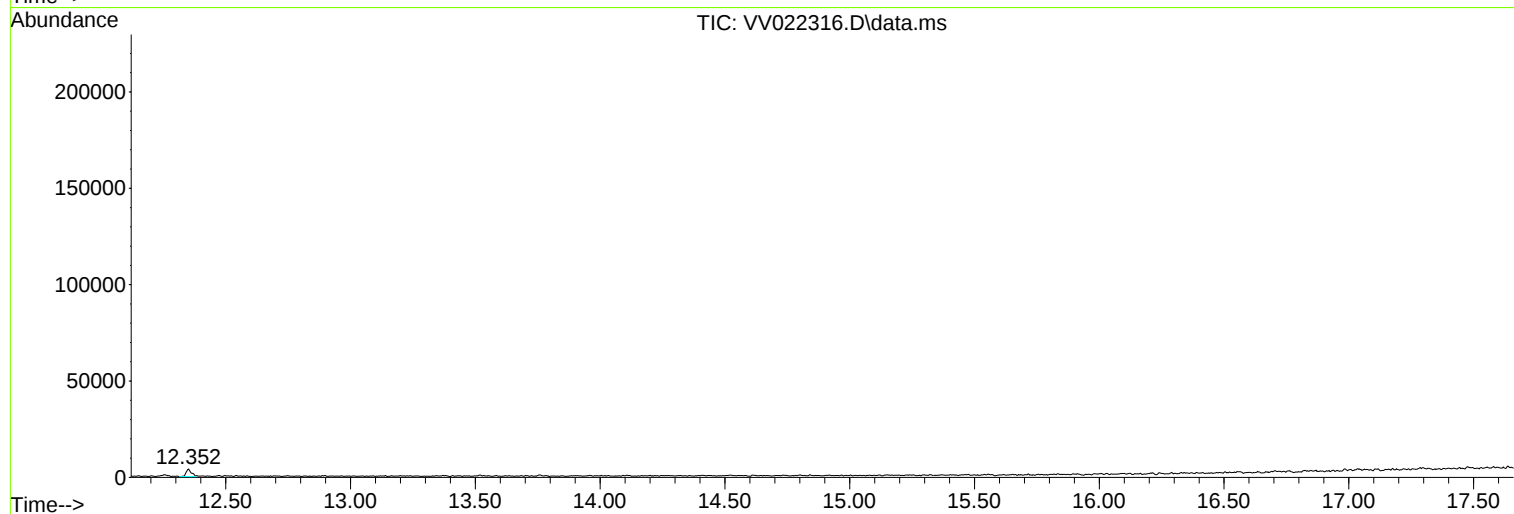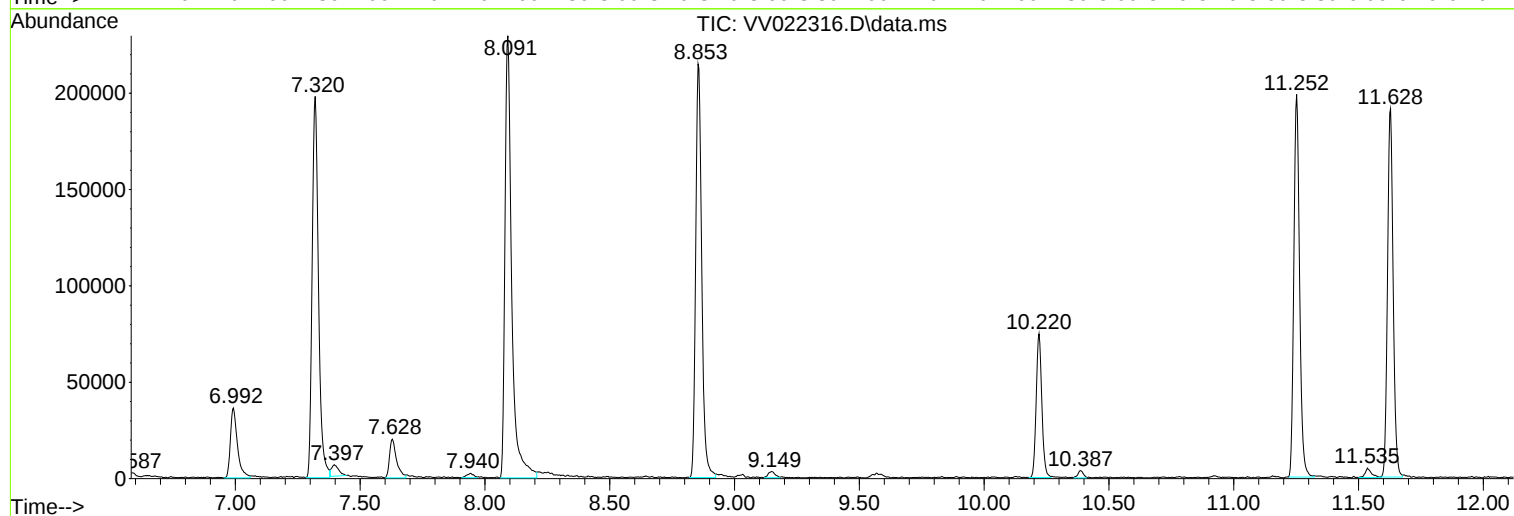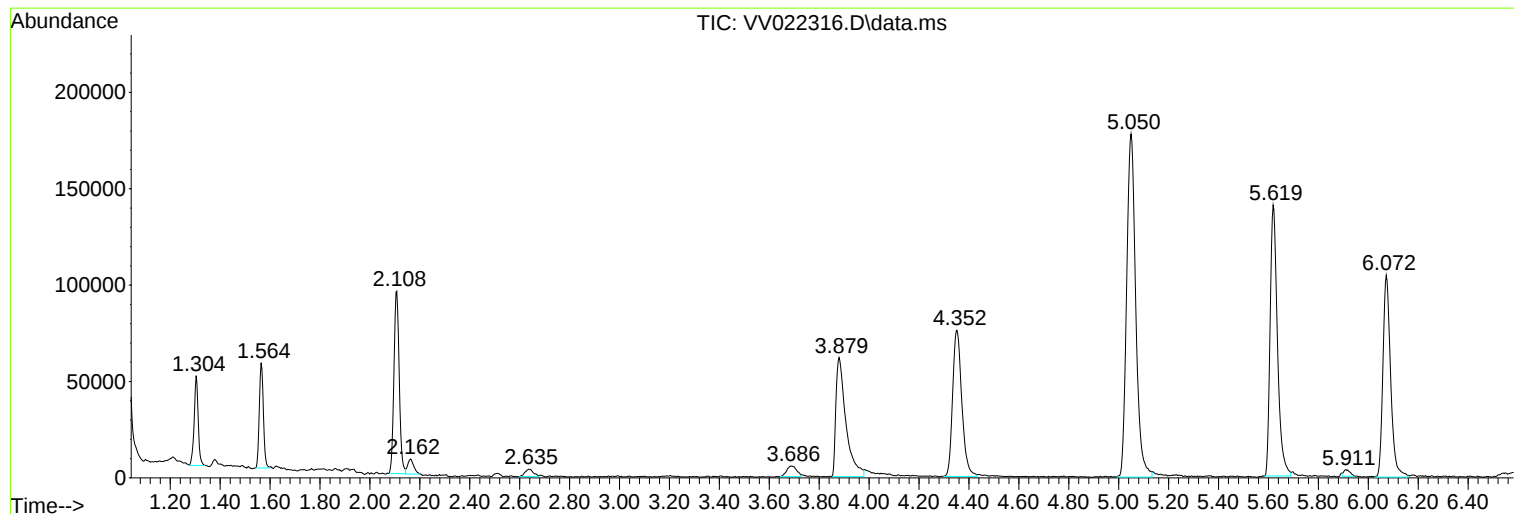

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022316.D
Acq On : 24 Sep 2021 12:36
Operator : SY/MD
Sample : M3814-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6X9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022316.D
Acq On : 24 Sep 2021 12:36
Operator : SY/MD
Sample : M3814-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6X9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
