

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
 Data File : VV022317.D
 Acq On : 24 Sep 2021 13:00
 Operator : SY/MD
 Sample : M3814-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6Y0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022317.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	95	rVB	47815	53651	11.96%	1.433%
2	1.564	156	163	173	rBV	55895	62728	13.99%	1.675%
3	2.105	321	331	342	rBV	95593	136841	30.51%	3.654%
4	2.191	349	358	383	rVB2	9678	32976	7.35%	0.881%
5	3.690	809	824	838	rBV5	6304	18716	4.17%	0.500%
6	3.908	880	892	936	rBV	46415	188038	41.93%	5.021%
7	4.352	1008	1030	1059	rBV	76717	195131	43.51%	5.211%
8	5.050	1232	1247	1277	rBV2	180580	448494	100.00%	11.976%
9	5.619	1410	1424	1452	rBV	145610	304693	67.94%	8.136%
10	5.911	1506	1515	1516	rBV4	3838	4727	1.05%	0.126%
11	6.072	1552	1565	1594	rBV	105652	221667	49.42%	5.919%
12	6.538	1702	1710	1717	rBV4	2502	4910	1.09%	0.131%
13	6.992	1839	1851	1870	rBV2	36098	70718	15.77%	1.888%
14	7.320	1942	1953	1970	rBV	194063	349571	77.94%	9.335%
15	7.628	2034	2049	2064	rBV2	22029	41077	9.16%	1.097%
16	8.091	2182	2193	2229	rBV	233619	446839	99.63%	11.932%
17	8.857	2418	2431	2458	rBV	221845	376903	84.04%	10.065%
18	10.220	2843	2855	2872	rBV	75649	119573	26.66%	3.193%
19	10.384	2897	2906	2916	rBV4	3796	6083	1.36%	0.162%
20	11.252	3163	3176	3197	rBV	212339	335526	74.81%	8.960%
21	11.535	3255	3264	3282	rBV3	10212	19762	4.41%	0.528%
22	11.628	3282	3293	3309	rBV	189387	306245	68.28%	8.178%




Sum of corrected areas: 3744869

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022317.D
Acq On : 24 Sep 2021 13:00
Operator : SY/MD
Sample : M3814-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

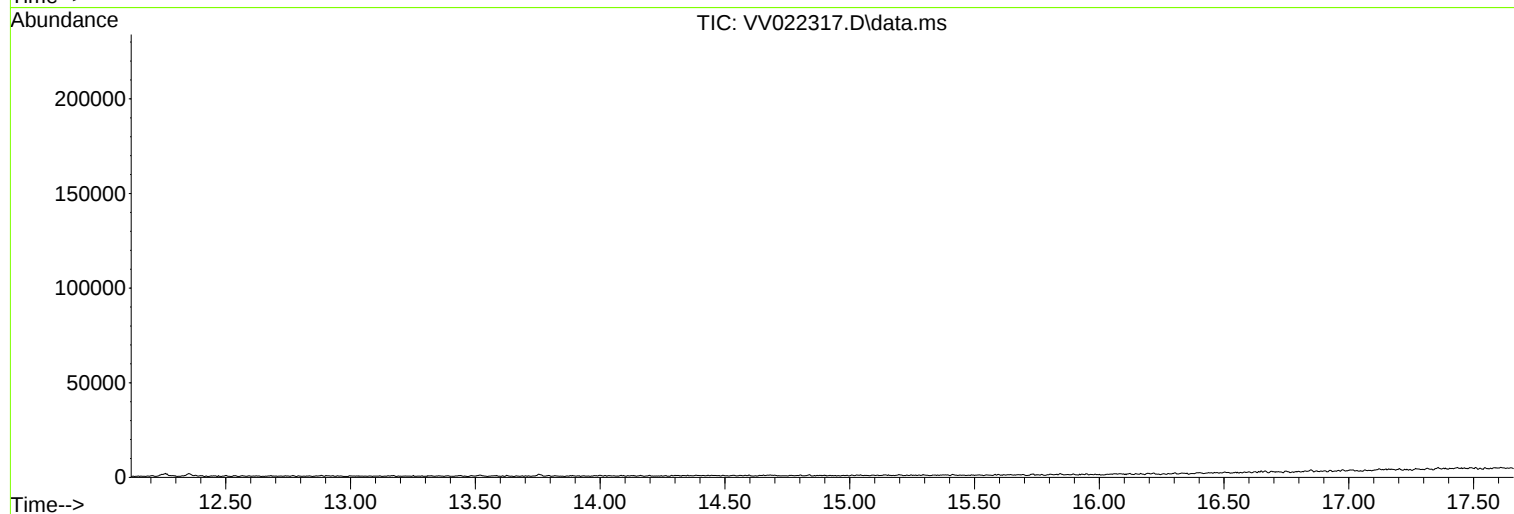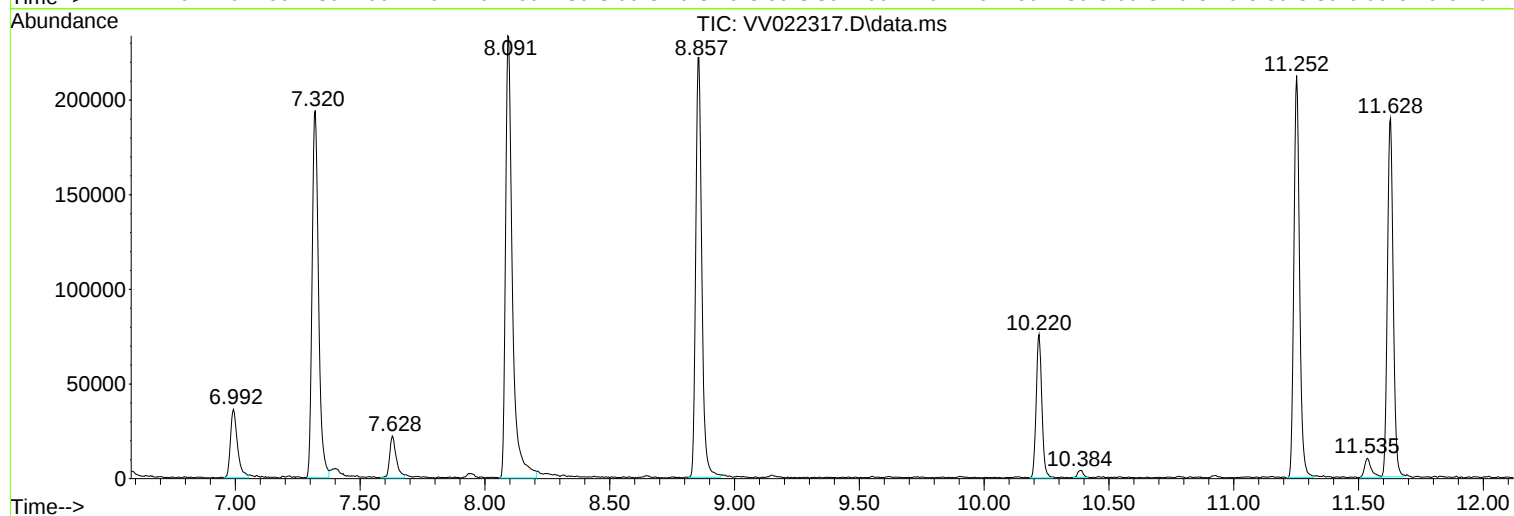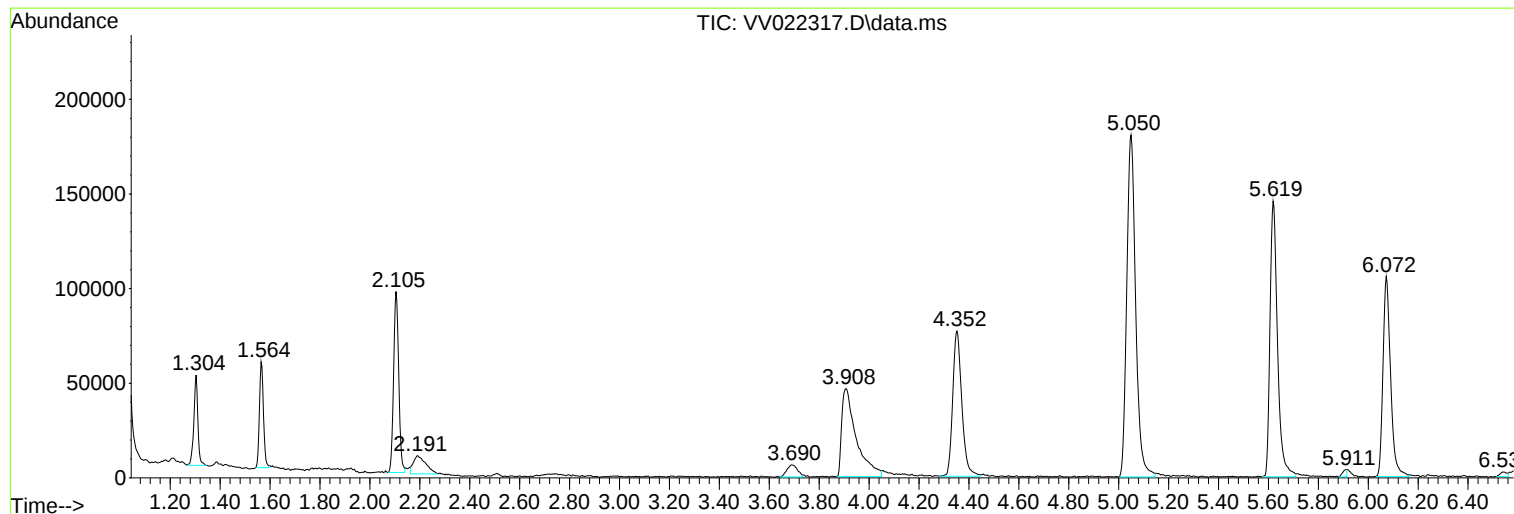

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022317.D
Acq On : 24 Sep 2021 13:00
Operator : SY/MD
Sample : M3814-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022317.D
Acq On : 24 Sep 2021 13:00
Operator : SY/MD
Sample : M3814-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6Y0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
