

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
 Data File : VV022318.D
 Acq On : 24 Sep 2021 13:36
 Operator : SY/MD
 Sample : M3814-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV022318.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	90	rVB	48493	48870	9.76%	1.247%
2	1.564	155	163	175	rBV	62629	73574	14.69%	1.878%
3	2.101	319	330	344	rBV	106961	155447	31.05%	3.967%
4	2.503	446	455	468	rBV	19254	32540	6.50%	0.830%
5	3.031	610	619	635	rVB7	4540	10154	2.03%	0.259%
6	3.908	878	892	920	rBV2	42815	175021	34.96%	4.466%
7	4.346	1013	1028	1051	rBV2	85688	215757	43.09%	5.506%
8	5.043	1229	1245	1276	rBV2	201269	500693	100.00%	12.777%
9	5.616	1411	1423	1450	rBV2	139408	293566	58.63%	7.491%
10	6.069	1549	1564	1591	rBV	115663	243601	48.65%	6.216%
11	6.989	1839	1850	1878	rBV	39961	78724	15.72%	2.009%
12	7.317	1940	1952	1973	rBV	215446	390462	77.98%	9.964%
13	7.394	1973	1976	1992	rVB7	3834	6607	1.32%	0.169%
14	7.625	2038	2048	2065	rBV2	23409	44619	8.91%	1.139%
15	8.091	2183	2193	2218	rBV	256251	488180	97.50%	12.458%
16	8.853	2419	2430	2453	rBV	217343	362907	72.48%	9.261%
17	10.217	2844	2854	2871	rVB	85207	134800	26.92%	3.440%
18	11.252	3165	3176	3198	rBV	200855	323259	64.56%	8.249%
19	11.625	3281	3292	3315	rBV	210808	339893	67.88%	8.674%




Sum of corrected areas: 3918674

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022318.D
Acq On : 24 Sep 2021 13:36
Operator : SY/MD
Sample : M3814-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

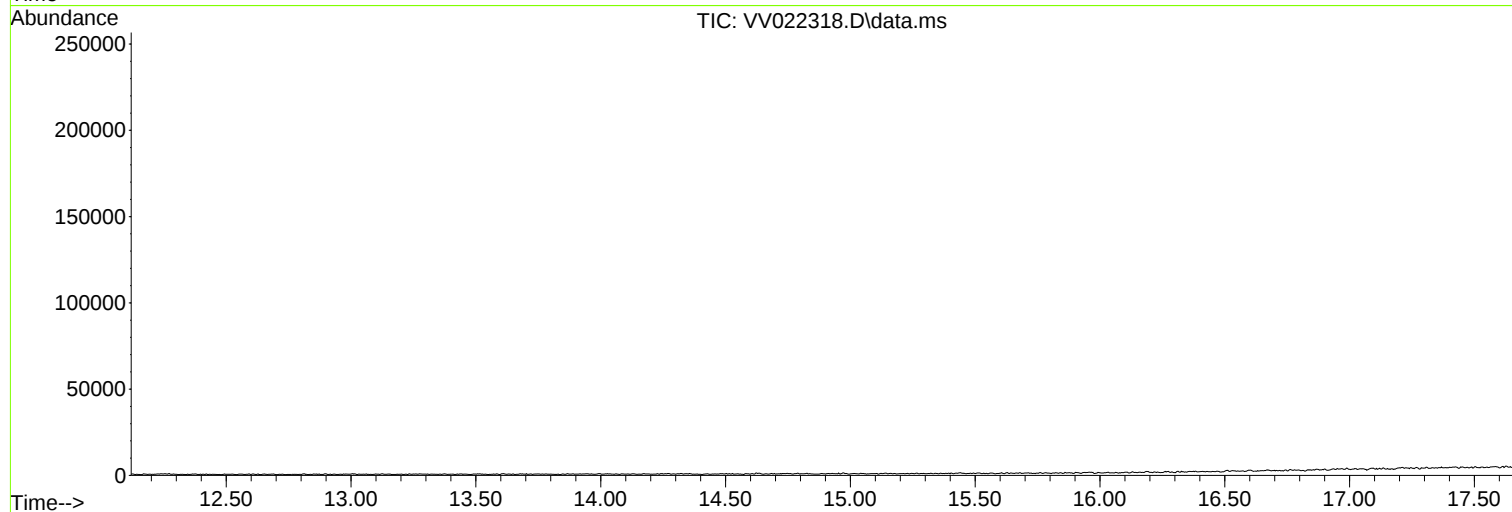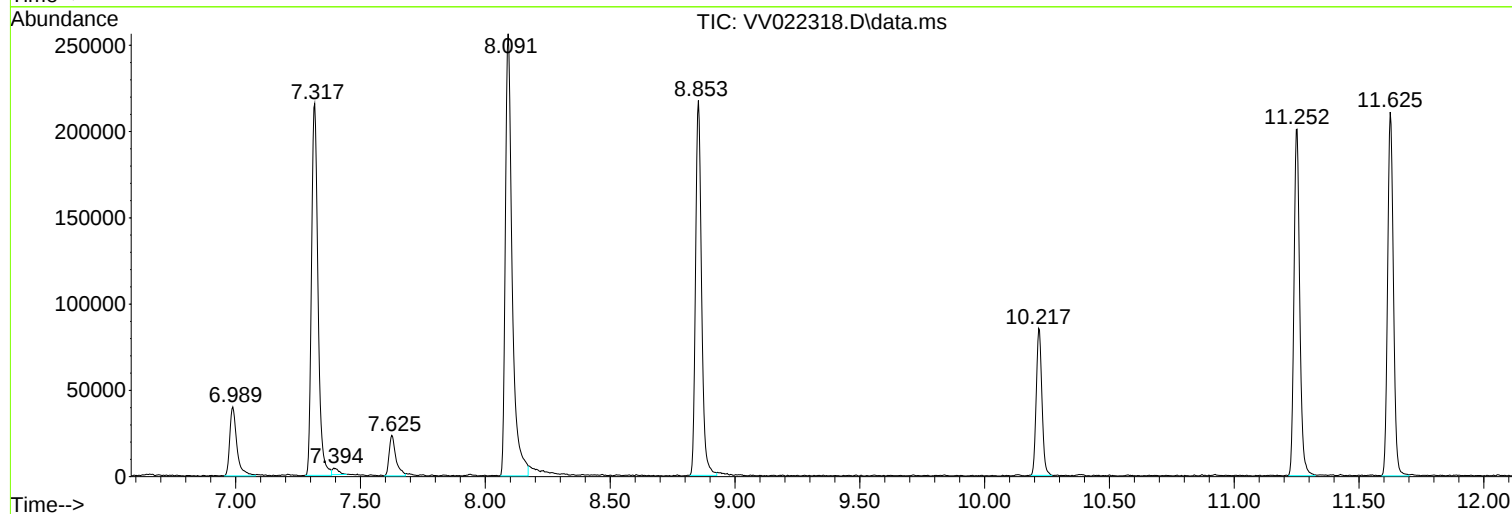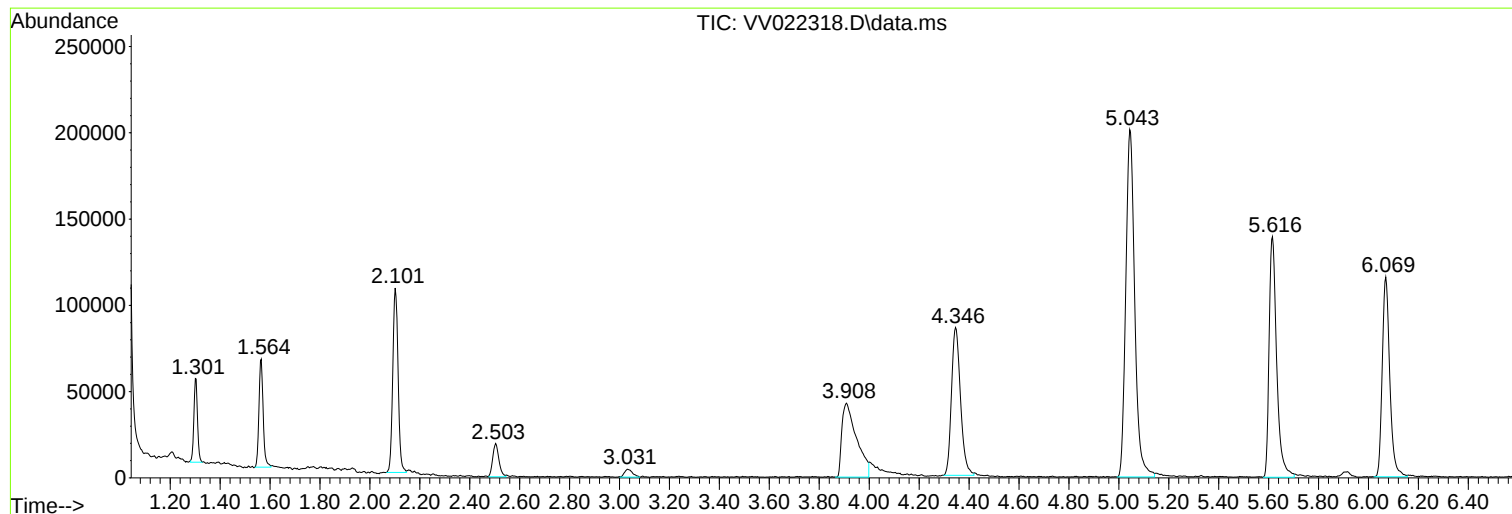

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022318.D
Acq On : 24 Sep 2021 13:36
Operator : SY/MD
Sample : M3814-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022318.D
Acq On : 24 Sep 2021 13:36
Operator : SY/MD
Sample : M3814-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
