

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
 Data File : VV022320.D
 Acq On : 24 Sep 2021 14:33
 Operator : SY/MD
 Sample : M3873-23
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW7Z0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV022320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	58	62	72	rVB	8344	11003	2.50%	0.302%
2	1.304	76	82	99	rVB	46770	49875	11.34%	1.371%
3	1.565	156	163	178	rBV	57730	66493	15.12%	1.828%
4	2.011	294	302	312	rBV9	2446	4606	1.05%	0.127%
5	2.105	321	331	342	rBV	95833	138700	31.54%	3.813%
6	2.163	342	349	366	rVB2	9990	20407	4.64%	0.561%
7	2.282	376	386	404	rVB3	4812	10910	2.48%	0.300%
8	2.507	442	456	469	rBV2	13604	24071	5.47%	0.662%
9	3.034	609	620	637	rBV6	3819	8848	2.01%	0.243%
10	3.873	870	881	914	rBV	58317	162820	37.02%	4.476%
11	4.346	1012	1028	1052	rBV2	76148	194547	44.24%	5.348%
12	5.047	1228	1246	1270	rBV2	174498	439768	100.00%	12.089%
13	5.616	1410	1423	1445	rBV	141531	291367	66.25%	8.010%
14	5.908	1504	1514	1523	rBV8	4087	7885	1.79%	0.217%
15	6.069	1551	1564	1587	rBV	101323	215015	48.89%	5.911%
16	6.989	1837	1850	1868	rBV	35841	68096	15.48%	1.872%
17	7.317	1939	1952	1970	rBV	190033	339258	77.14%	9.326%
18	7.394	1974	1976	1987	rVB5	3532	4798	1.09%	0.132%
19	7.625	2038	2048	2065	rBV	20394	38650	8.79%	1.063%
20	7.789	2088	2099	2112	rBV2	15534	28303	6.44%	0.778%
21	8.088	2182	2192	2225	rBV	214091	401710	91.35%	11.043%
22	8.799	2400	2413	2419	rBV5	4364	7725	1.76%	0.212%
23	8.854	2419	2430	2453	rVV	219489	361355	82.17%	9.934%
24	10.217	2844	2854	2869	rBV	70936	110708	25.17%	3.043%
25	11.066	3107	3118	3129	rBV8	2864	4969	1.13%	0.137%
26	11.252	3164	3176	3193	rBV	204462	322461	73.33%	8.865%
27	11.538	3257	3265	3278	rBV6	3406	6678	1.52%	0.184%
28	11.625	3281	3292	3308	rBV	184910	296614	67.45%	8.154%




Sum of corrected areas: 3637640

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022320.D
Acq On : 24 Sep 2021 14:33
Operator : SY/MD
Sample : M3873-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

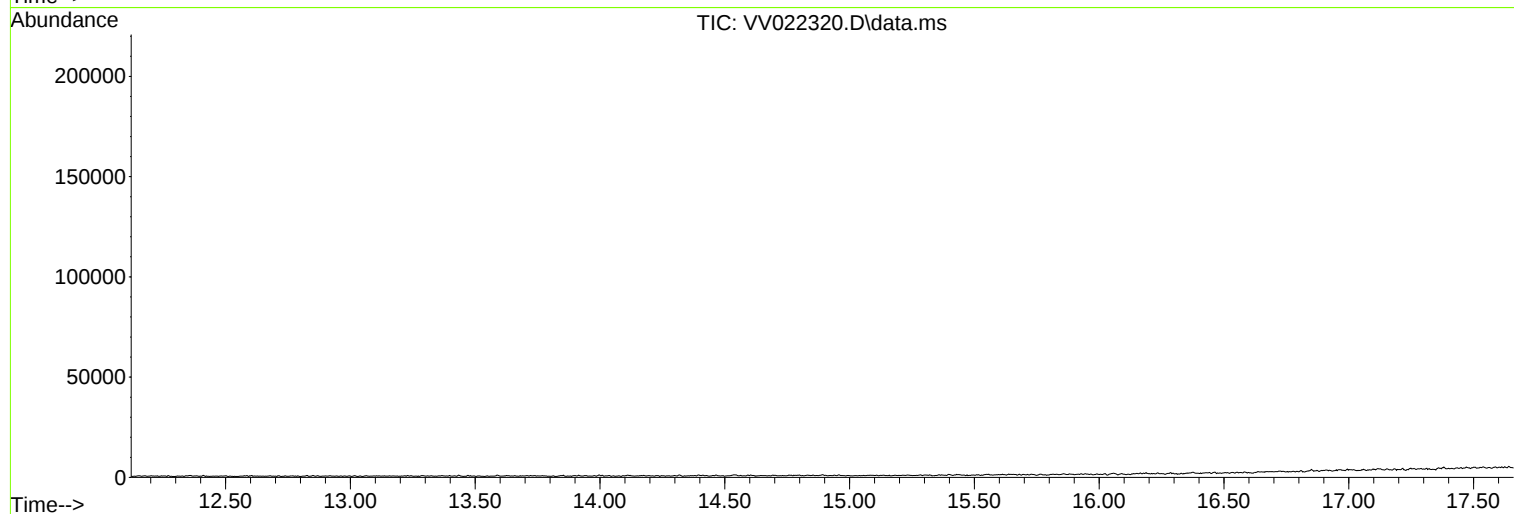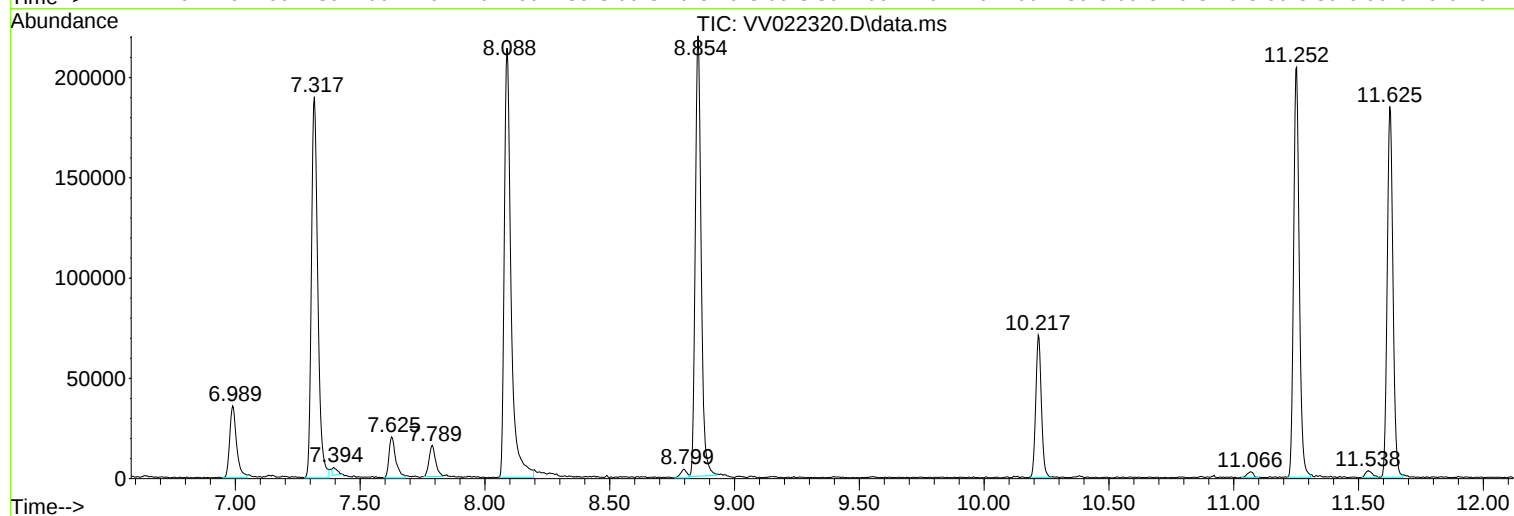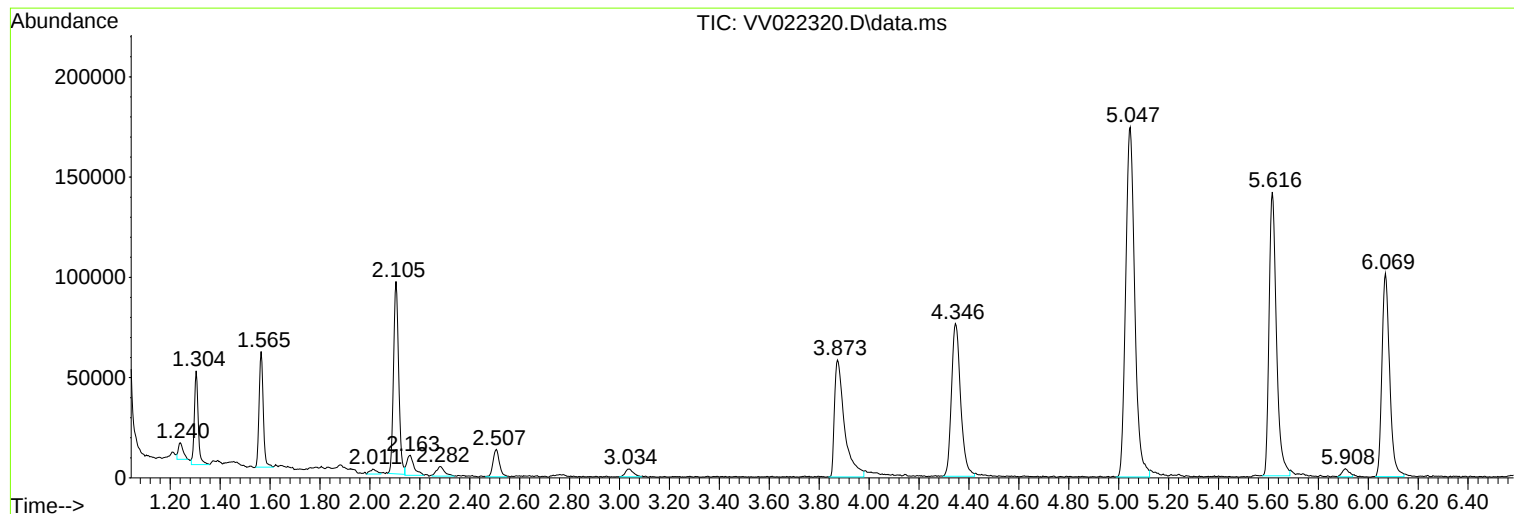

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022320.D
Acq On : 24 Sep 2021 14:33
Operator : SY/MD
Sample : M3873-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
Data File : VV022320.D
Acq On : 24 Sep 2021 14:33
Operator : SY/MD
Sample : M3873-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW7Z0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
