
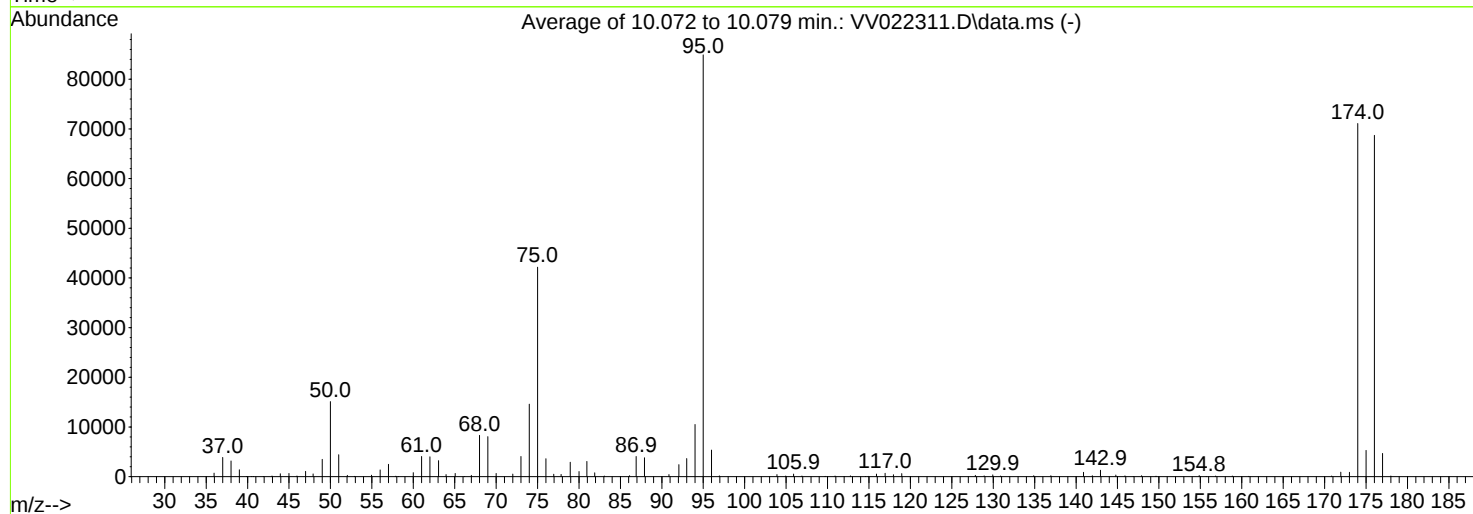


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092421\
 Data File : VV022311.D
 Acq On : 24 Sep 2021 09:29
 Operator : SY/MD
 Sample : BFB206
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB206

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Sep 25 04:30:06 2021

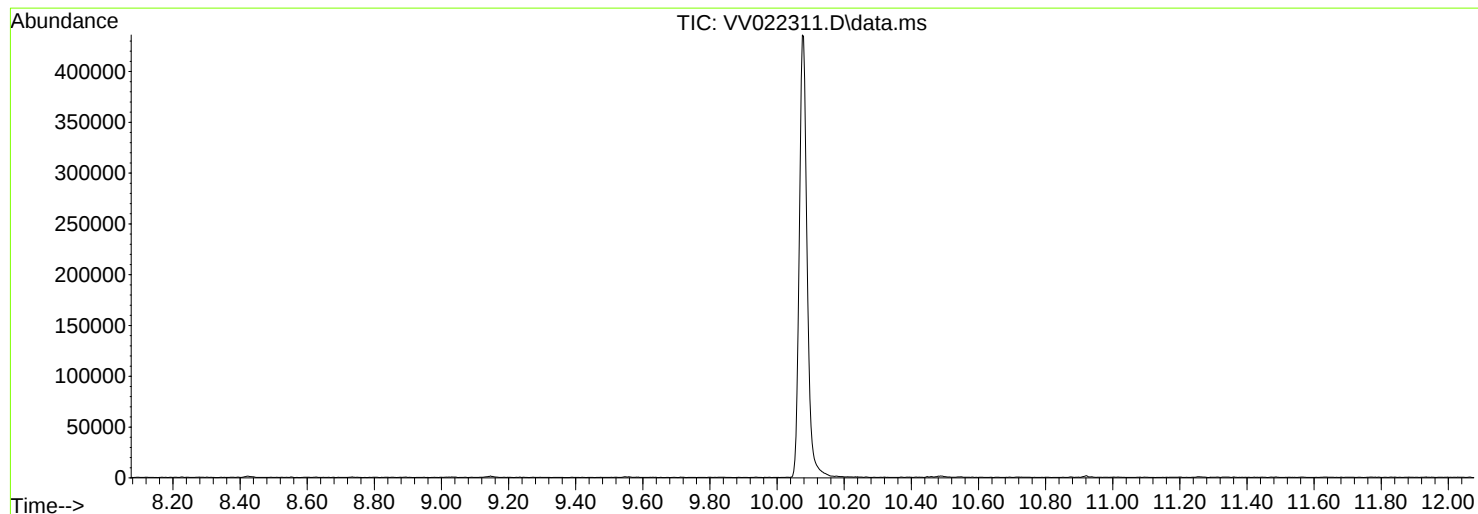

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	15120	PASS
75	95	30	80	49.6	42144	PASS
95	95	100	100	100.0	84904	PASS
96	95	5	9	6.3	5363	PASS
173	174	0.00	2	1.2	883	PASS
174	95	50	120	83.7	71085	PASS
175	174	5	9	7.4	5289	PASS
176	174	95	105	96.7	68704	PASS
177	176	5	10	6.8	4678	PASS

m/z	Abundance
35.80	112.0
40.00	188.0
43.90	271.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	748.0
37.00	3673.0
38.00	2994.0
39.00	1352.0
39.90	202.0
41.90	130.0
42.90	115.0
44.00	793.0
45.00	682.0
46.00	143.0
47.00	975.0
47.90	489.0
49.00	3492.0
50.00	14519.0
51.00	4333.0
52.10	238.0
52.90	101.0
54.90	261.0
56.00	1337.0
57.00	2359.0
58.20	116.0
60.00	733.0
61.00	3930.0
62.00	3921.0
63.10	2946.0
63.90	333.0
65.10	655.0
67.00	222.0
68.00	7791.0
69.00	7628.0
70.00	626.0
72.00	471.0
73.00	3854.0
74.00	13708.0
75.00	39944.0
76.00	3475.0
77.00	462.0
77.80	444.0
79.00	2751.0
80.00	968.0
80.90	2979.0
81.90	764.0
83.10	104.0
86.10	221.0
86.90	3775.0
87.90	3753.0
90.90	390.0
92.00	2315.0
93.00	3469.0
94.00	9845.0
95.00	78928.0
96.00	5236.0
97.00	189.0
103.90	423.0
105.00	118.0
105.90	461.0
106.90	126.0
110.90	119.0
112.80	180.0
114.90	112.0
115.90	513.0
117.00	661.0
117.90	400.0
118.90	514.0
127.80	269.0
129.00	170.0
130.00	311.0
130.90	140.0
134.90	174.0
137.00	208.0
140.90	889.0
142.00	143.0
142.90	1179.0
144.80	294.0
145.90	116.0
146.90	103.0
147.90	153.0
154.90	219.0
156.90	142.0
158.80	108.0
160.80	112.0
171.00	142.0
172.00	841.0
173.00	943.0
174.00	65064.0
175.00	4818.0
176.00	61968.0
177.00	4506.0
178.00	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	869.0
37.00	4044.0
38.00	3211.0
39.00	1425.0
39.90	220.0
40.50	115.0
42.90	112.0
44.00	883.0
45.00	680.0
45.90	149.0
47.00	1089.0
47.90	579.0
49.00	3599.0
50.00	15578.0
51.00	4527.0
52.00	258.0
52.90	101.0
55.00	292.0
56.00	1430.0
57.00	2582.0
57.90	126.0
60.00	830.0
61.00	4193.0
62.00	4161.0
63.00	3345.0
64.00	439.0
65.10	675.0
66.20	104.0
67.00	276.0
68.00	8634.0
69.00	8301.0
70.00	649.0
72.00	539.0
73.00	4257.0
74.00	15105.0
75.00	43616.0
76.00	3742.0
76.90	478.0
77.80	472.0
79.00	3057.0
80.00	1082.0
80.90	3171.0
81.90	756.0
83.00	128.0
86.10	226.0
86.90	4190.0
87.90	3970.0
90.90	420.0
92.00	2423.0
93.00	3785.0
94.00	10919.0
95.00	88072.0
96.00	5491.0
97.00	170.0
103.90	430.0
105.00	160.0
105.90	562.0
106.90	130.0
109.70	104.0
110.90	141.0
112.80	175.0
114.90	107.0
115.90	542.0
116.90	673.0
117.90	409.0
119.00	633.0
127.80	250.0
128.90	191.0
129.90	364.0
130.90	149.0
134.90	220.0
136.90	207.0
140.90	878.0
142.00	192.0
142.90	1350.0
144.80	323.0
145.90	173.0
147.90	200.0
149.60	124.0
154.80	244.0
156.90	141.0
158.80	143.0
160.90	111.0
170.80	143.0
172.00	909.0
173.00	905.0
174.00	73624.0
175.00	5482.0
176.00	71008.0
177.00	4831.0
178.00	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206

m/z	Abundance
36.00	829.0
37.00	3857.0
38.00	3282.0
39.00	1409.0
39.90	221.0
40.70	133.0
43.00	120.0
44.00	855.0
45.00	619.0
45.90	148.0
47.00	1100.0
47.90	621.0
49.00	3382.0
50.00	15263.0
51.00	4366.0
52.00	280.0
55.00	279.0
56.00	1329.0
57.00	2490.0
57.90	133.0
60.00	841.0
61.00	4073.0
62.00	3882.0
63.00	3375.0
64.00	455.0
65.00	638.0
67.00	308.0
68.00	8481.0
69.00	8280.0
70.00	621.0
72.00	536.0
73.00	4055.0
74.00	14979.0
75.00	42872.0
76.00	3598.0
76.90	505.0
77.90	440.0
78.90	2905.0
80.00	1074.0
81.00	3029.0
81.90	772.0
83.00	136.0
86.10	180.0
86.90	4206.0
87.90	3709.0
90.80	402.0
92.10	2499.0
93.00	3711.0
94.00	10786.0
95.00	87712.0
96.00	5363.0
96.90	143.0
103.90	410.0
104.90	161.0
105.90	568.0
106.90	115.0
109.70	110.0
110.90	147.0
112.00	105.0
112.70	158.0
114.60	117.0
115.90	483.0
116.90	670.0
118.00	395.0
119.00	659.0
127.90	225.0
128.80	165.0
129.90	370.0
130.90	127.0
134.90	233.0
136.90	183.0
140.90	867.0
141.90	212.0
143.00	1346.0
144.80	317.0
145.90	196.0
147.90	220.0
149.70	161.0
154.80	254.0
155.70	111.0
156.80	158.0
158.90	167.0
170.70	131.0
171.90	958.0
173.00	800.0
174.00	74568.0
175.00	5567.0
176.00	73136.0
177.00	4698.0
178.00	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB206