

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092424\
 Data File : VV037500.D
 Acq On : 24 Sep 2024 12:27
 Operator : SY/MD
 Sample : P3994-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV037500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	64	73	91	rVV	146690	165064	11.70%	1.517%
2	1.529	145	152	166	rVB	139626	163613	11.59%	1.504%
3	2.053	305	315	332	rVB	270268	396037	28.06%	3.640%
4	2.446	428	437	447	rBV3	11507	20718	1.47%	0.190%
5	3.812	852	862	911	rBV	119210	491771	34.84%	4.520%
6	4.243	980	996	1024	rBV	202512	537825	38.11%	4.943%
7	4.950	1202	1216	1250	rBV2	486655	1249053	88.50%	11.480%
8	5.529	1383	1396	1435	rBV	378042	844817	59.86%	7.765%
9	5.982	1525	1537	1564	rBV	276247	600491	42.55%	5.519%
10	6.915	1815	1827	1853	rBV	115231	249203	17.66%	2.290%
11	7.240	1917	1928	1967	rBV	562895	1077663	76.36%	9.905%
12	7.558	2018	2027	2050	rBV	62852	137776	9.76%	1.266%
13	8.024	2163	2172	2232	rBV	621288	1411357	100.00%	12.972%
14	8.780	2397	2407	2434	rBV	606784	1056953	74.89%	9.714%
15	10.149	2823	2833	2857	rBV	227509	379542	26.89%	3.488%
16	10.317	2870	2885	2897	rVB9	7227	16004	1.13%	0.147%
17	11.181	3143	3154	3186	rBV	621299	1059290	75.05%	9.736%
18	11.554	3260	3270	3296	rBV	593962	983732	69.70%	9.041%
19	13.448	3850	3859	3877	rBV2	17597	39416	2.79%	0.362%




Sum of corrected areas: 10880325

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092424\
Data File : VV037500.D
Acq On : 24 Sep 2024 12:27
Operator : SY/MD
Sample : P3994-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

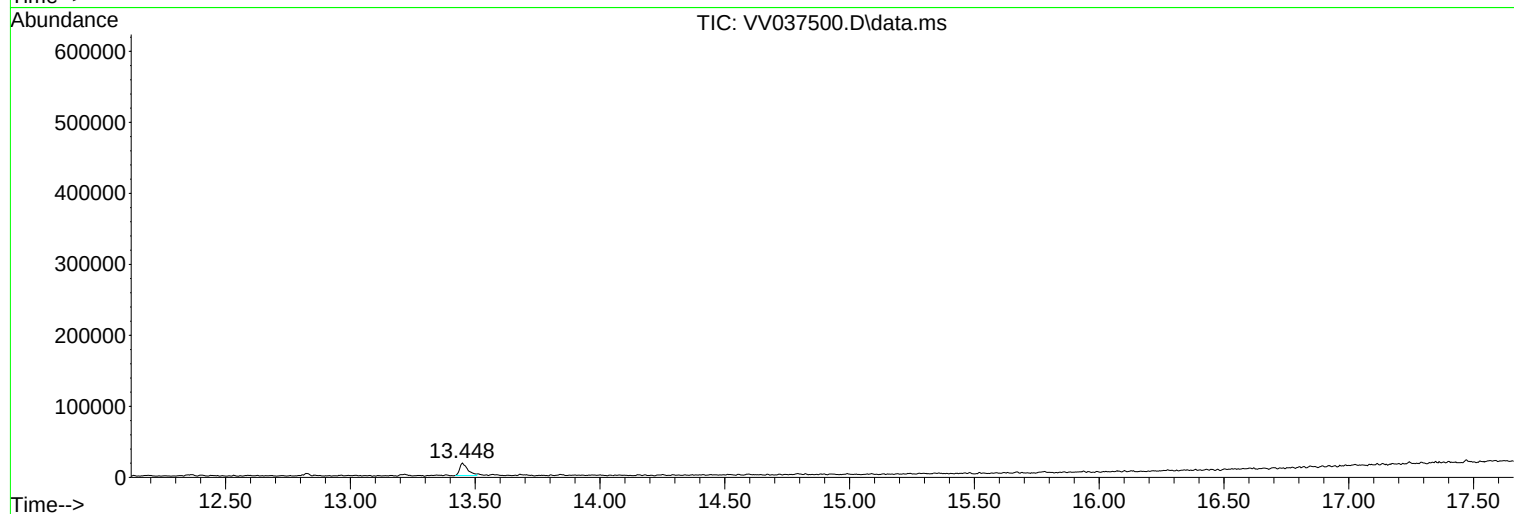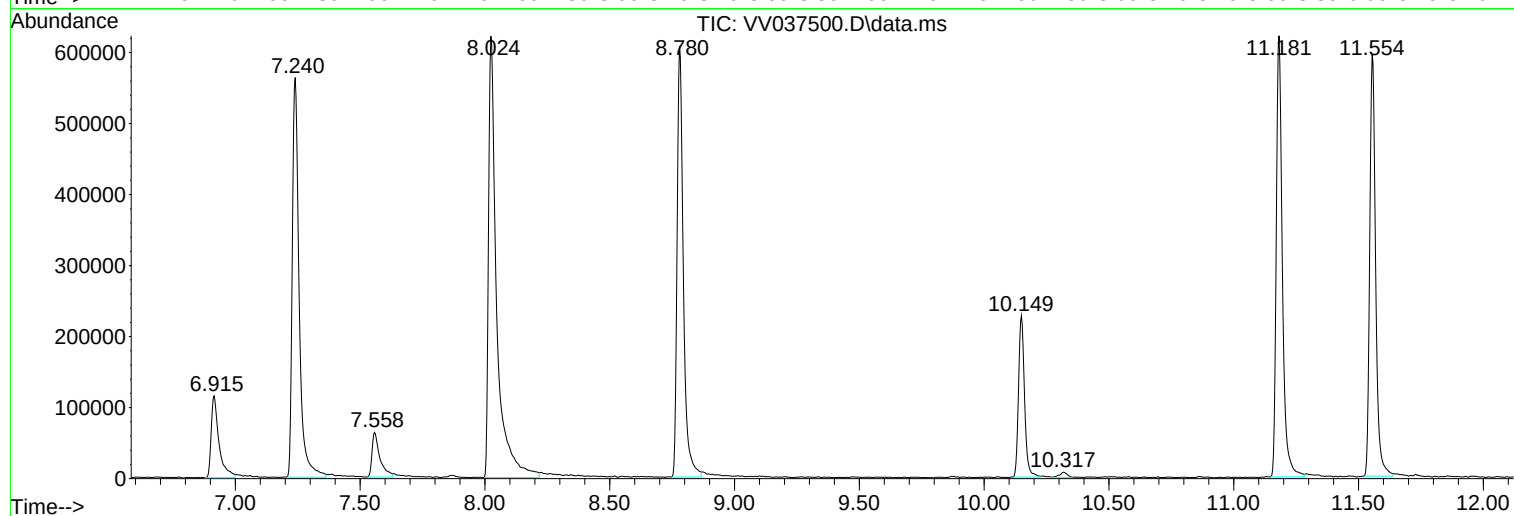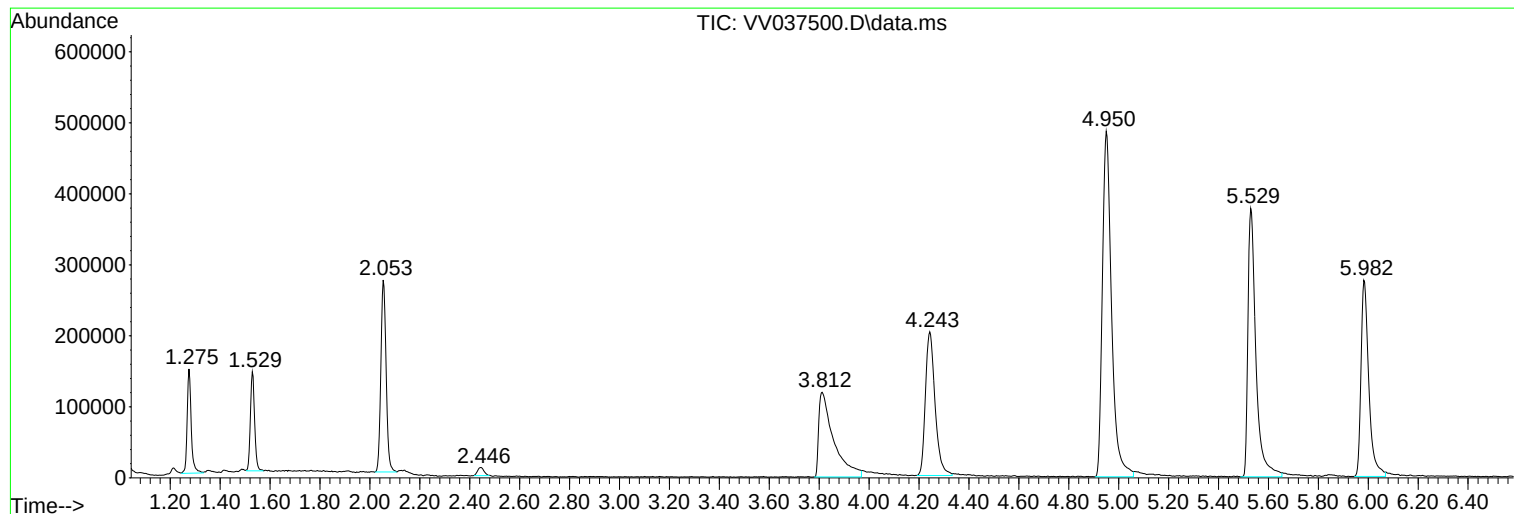

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092424\
Data File : VV037500.D
Acq On : 24 Sep 2024 12:27
Operator : SY/MD
Sample : P3994-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092424\
Data File : VV037500.D
Acq On : 24 Sep 2024 12:27
Operator : SY/MD
Sample : P3994-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc