

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092424\
 Data File : VV037503.D
 Acq On : 24 Sep 2024 13:42
 Operator : SY/MD
 Sample : VIBLK387
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK387

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV037503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	65	73	86	rBV	127616	139663	10.95%	1.361%
2	1.529	144	152	163	rBV	122860	144507	11.33%	1.409%
3	2.053	305	315	331	rVB	234388	339150	26.59%	3.306%
4	2.442	428	436	449	rVB4	7625	13357	1.05%	0.130%
5	3.825	852	866	904	rBV3	107330	521914	40.91%	5.087%
6	4.243	977	996	1025	rBV	179989	482554	37.83%	4.704%
7	4.950	1202	1216	1249	rBV2	424950	1113084	87.26%	10.849%
8	5.529	1384	1396	1430	rBV	417427	910032	71.34%	8.870%
9	5.982	1524	1537	1565	rBV	238657	531731	41.68%	5.183%
10	6.915	1815	1827	1850	rBV	98099	214561	16.82%	2.091%
11	7.240	1916	1928	1957	rBV	482096	921529	72.24%	8.982%
12	7.558	2017	2027	2052	rBV2	52506	118922	9.32%	1.159%
13	8.027	2161	2173	2226	rBV	539232	1275665	100.00%	12.434%
14	8.365	2269	2278	2295	rVB4	8665	18066	1.42%	0.176%
15	8.780	2396	2407	2435	rBV	662432	1143318	89.63%	11.144%
16	10.149	2819	2833	2852	rBV	209317	348985	27.36%	3.402%
17	10.317	2876	2885	2898	rVB3	7885	14867	1.17%	0.145%
18	11.182	3143	3154	3183	rBV	665870	1134390	88.93%	11.057%
19	11.555	3258	3270	3297	rBV	521066	873026	68.44%	8.510%




Sum of corrected areas: 10259321

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092424\
Data File : VV037503.D
Acq On : 24 Sep 2024 13:42
Operator : SY/MD
Sample : VIBLK387
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK387

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

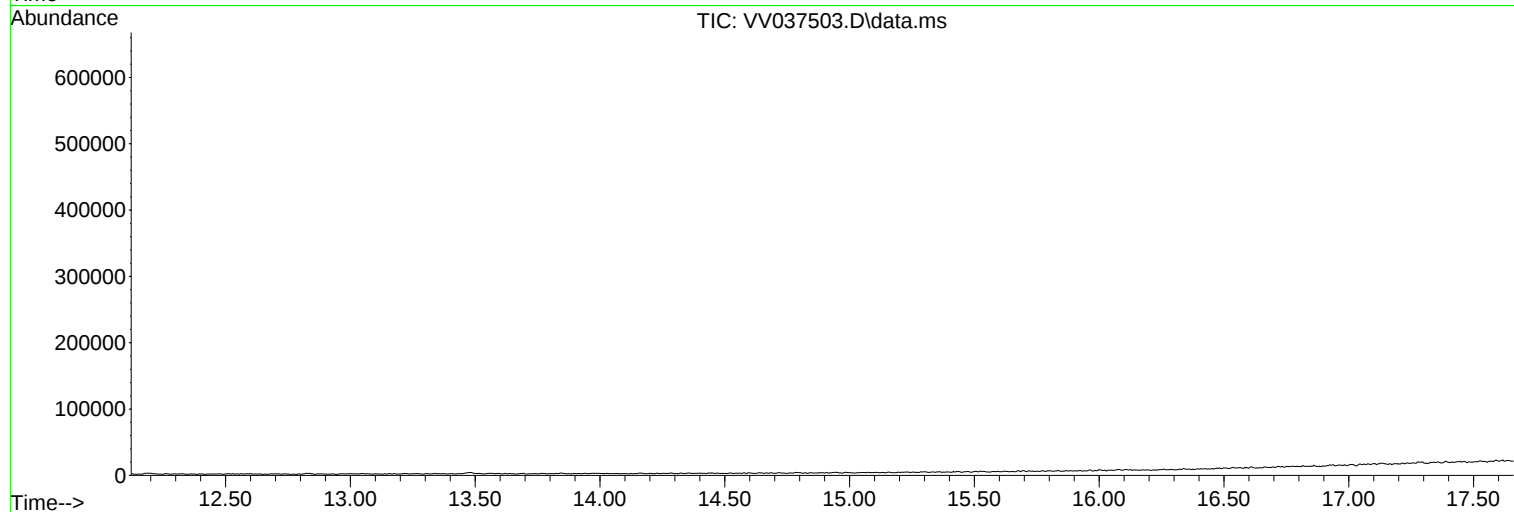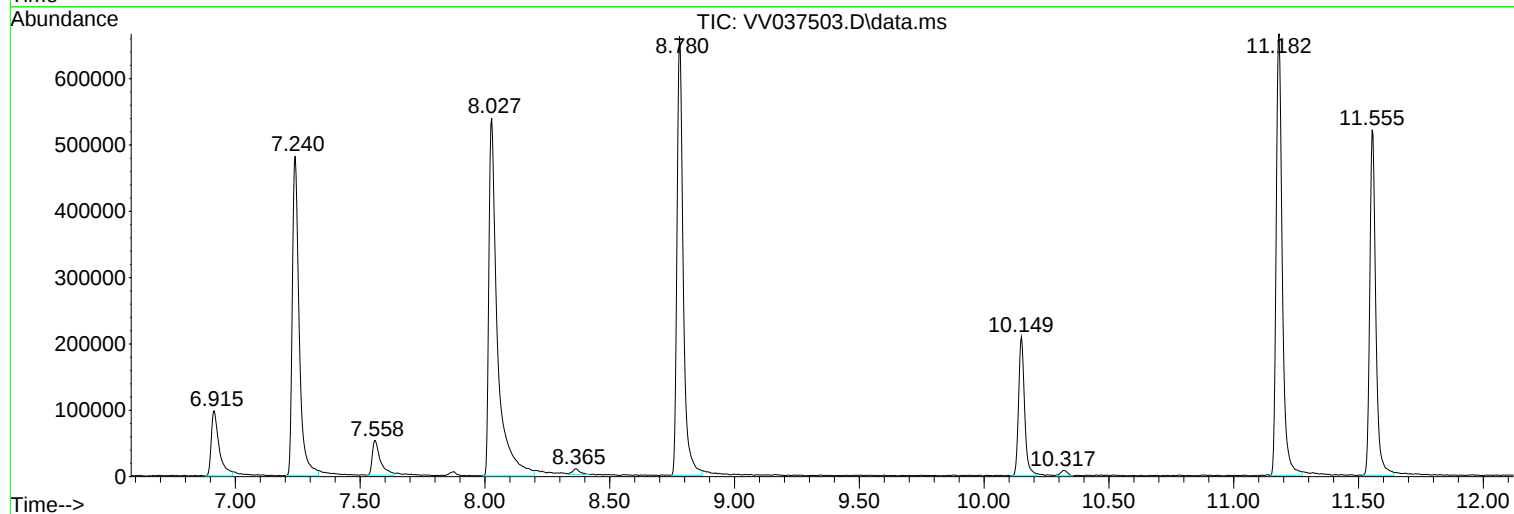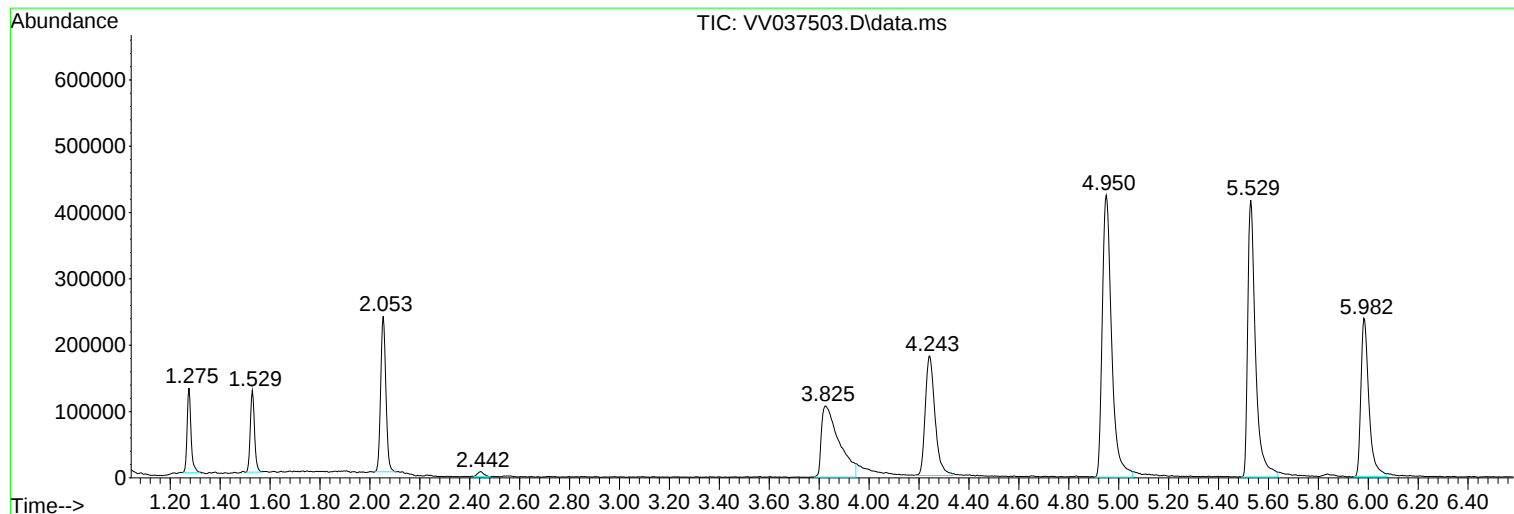

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092424\
Data File : VV037503.D
Acq On : 24 Sep 2024 13:42
Operator : SY/MD
Sample : VIBLK387
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK387

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092424\
Data File : VV037503.D
Acq On : 24 Sep 2024 13:42
Operator : SY/MD
Sample : VIBLK387
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK387

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc