
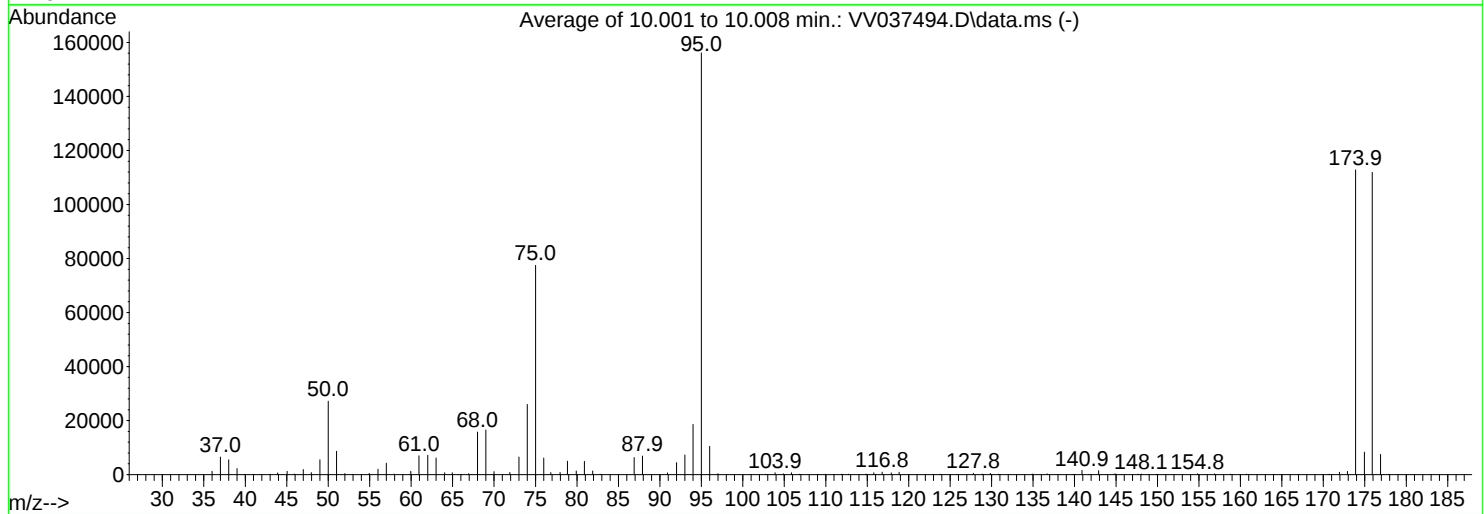


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092424\
Data File : VV037494.D
Acq On : 24 Sep 2024 08:43
Operator : SY/MD
Sample : BFB278
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB278

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 25 02:58:03 2024

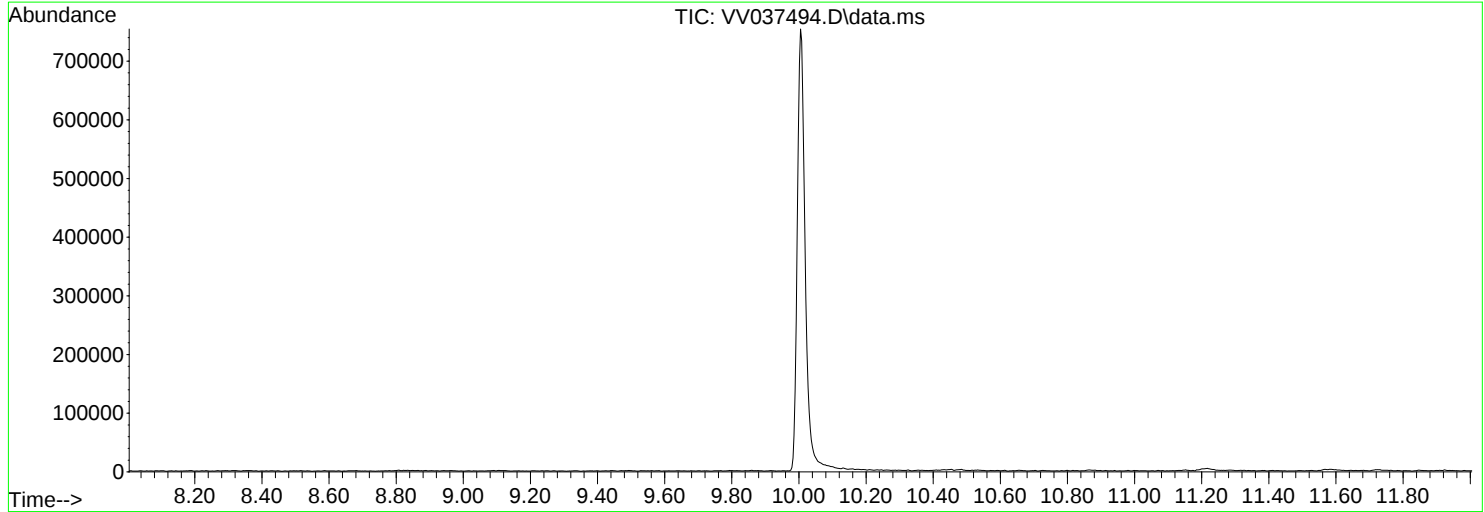

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	27163	PASS
75	95	30	80	49.6	77477	PASS
95	95	100	100	100.0	156139	PASS
96	95	5	9	6.7	10475	PASS
173	174	0.00	2	1.1	1200	PASS
174	95	50	120	72.3	112832	PASS
175	174	5	9	7.4	8340	PASS
176	174	95	105	99.2	111896	PASS
177	176	5	10	6.7	7480	PASS

m/z	Abundance
39.90	408.0
40.90	102.0
43.90	893.0
76.80	165.0
90.60	105.0
207.00	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278

m/z	Abundance
36.00	1138.0
37.00	6143.0
38.00	5425.0
39.00	2117.0
39.80	450.0
43.00	167.0
43.90	1758.0
45.10	1308.0
45.90	212.0
47.00	1667.0
47.90	768.0
49.00	5562.0
50.00	27064.0
51.00	8468.0
52.00	443.0
53.00	171.0
54.90	468.0
56.00	1898.0
57.00	3882.0
57.90	241.0
60.00	1224.0
60.90	6641.0
62.00	6858.0
63.00	5911.0
64.10	682.0
65.00	737.0
65.70	109.0
66.10	101.0
66.90	367.0
68.00	15604.0
69.00	15888.0
70.00	1242.0
71.90	780.0
73.00	6220.0
74.00	25728.0
75.00	74408.0
76.00	6234.0
76.90	912.0
78.00	916.0
78.90	4879.0
79.90	1313.0
80.90	4920.0
81.90	1350.0
82.80	186.0
86.10	189.0
86.90	6658.0
87.90	6613.0
90.90	648.0
92.00	4166.0
93.00	7191.0
94.00	17640.0
95.00	149696.0
96.00	10346.0
97.10	368.0
102.80	163.0
103.90	588.0
104.90	301.0
105.90	728.0
106.80	139.0
110.00	243.0
110.90	174.0
111.90	159.0
112.70	128.0
114.90	177.0
115.80	689.0
116.80	994.0
117.90	624.0
118.90	845.0
123.90	134.0
127.80	547.0
128.80	219.0
129.80	495.0
130.90	205.0
134.90	289.0
136.70	253.0
139.80	186.0
140.90	1586.0
142.00	195.0
142.90	1293.0
144.90	339.0
145.70	114.0
146.10	134.0
146.90	128.0
147.70	223.0
148.00	233.0
148.80	146.0
149.90	138.0
155.00	322.0
156.90	263.0
158.80	188.0
160.80	185.0
170.60	182.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278

171.90	870.0
172.90	1099.0
173.90	104704.0
175.00	8100.0
175.90	103696.0
176.90	7180.0
177.90	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278

m/z	Abundance
36.00	1273.0
37.00	6782.0
38.00	5662.0
39.00	2346.0
39.80	521.0
43.00	186.0
43.90	1567.0
45.00	1217.0
45.90	280.0
47.00	1993.0
47.90	788.0
49.00	5594.0
50.00	28072.0
51.00	9057.0
52.00	411.0
52.90	141.0
55.00	516.0
56.00	2071.0
57.00	4398.0
58.00	224.0
59.00	129.0
60.00	1281.0
60.90	7285.0
62.00	7380.0
63.00	6415.0
64.00	683.0
65.00	747.0
66.90	409.0
68.00	16300.0
69.00	17288.0
70.00	1159.0
71.90	826.0
73.00	6683.0
74.00	26816.0
75.00	80208.0
76.00	6315.0
76.90	905.0
77.90	856.0
78.90	5195.0
79.90	1424.0
80.90	5063.0
81.90	1390.0
82.80	222.0
86.00	130.0
86.90	6658.0
87.90	7216.0
90.90	692.0
92.00	4620.0
93.00	7609.0
94.00	19384.0
95.00	161792.0
96.00	10919.0
97.00	354.0
102.80	207.0
103.90	737.0
104.90	317.0
105.80	713.0
106.80	195.0
109.90	181.0
110.90	156.0
111.90	232.0
112.80	190.0
114.80	219.0
115.80	792.0
116.80	1009.0
117.90	707.0
118.90	951.0
123.80	196.0
127.80	575.0
128.80	253.0
129.90	522.0
130.80	224.0
134.90	273.0
136.70	290.0
140.00	173.0
140.90	1680.0
141.90	187.0
142.90	1573.0
144.90	404.0
146.00	152.0
147.00	145.0
147.70	212.0
148.10	262.0
148.80	137.0
149.80	160.0
154.00	106.0
154.80	377.0
156.90	322.0
158.70	173.0
160.70	196.0
170.70	153.0
172.00	907.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278

172.90	1231.0
173.90	116992.0
175.00	8588.0
175.90	116312.0
176.90	7738.0
177.90	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278

m/z	Abundance
36.00	1349.0
37.00	6619.0
38.00	5487.0
39.00	2352.0
39.90	539.0
41.80	171.0
43.00	184.0
44.00	1328.0
45.00	1159.0
46.00	244.0
47.00	2015.0
48.00	764.0
49.00	5311.0
50.00	26352.0
51.00	8405.0
52.00	364.0
52.90	131.0
55.00	522.0
56.00	2024.0
57.00	4529.0
58.00	183.0
59.00	131.0
59.90	1291.0
61.00	7047.0
62.00	7270.0
63.00	6200.0
64.00	724.0
64.90	742.0
67.00	389.0
68.00	15358.0
69.00	16377.0
70.00	937.0
71.90	833.0
73.00	6737.0
74.00	25480.0
75.00	77816.0
76.00	5997.0
76.90	920.0
77.90	735.0
78.80	4825.0
79.90	1430.0
80.90	4838.0
81.90	1297.0
82.80	151.0
85.90	107.0
86.90	5790.0
87.90	6750.0
90.90	648.0
92.00	4502.0
93.00	7125.0
94.00	18808.0
95.00	156928.0
96.00	10159.0
96.90	377.0
102.80	165.0
103.90	881.0
104.90	253.0
105.90	700.0
106.80	214.0
109.90	109.0
111.00	117.0
111.90	233.0
112.80	253.0
114.80	262.0
115.80	748.0
116.80	896.0
117.90	626.0
118.80	919.0
123.70	219.0
125.80	116.0
127.80	547.0
128.90	256.0
129.90	508.0
130.80	207.0
134.90	226.0
136.70	283.0
140.10	173.0
140.90	1527.0
141.70	196.0
142.90	1620.0
143.70	166.0
144.90	384.0
146.00	157.0
147.00	107.0
147.60	194.0
148.10	237.0
148.90	109.0
149.90	155.0
154.00	121.0
154.80	390.0
156.90	359.0
158.90	136.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278

160.70	182.0
170.80	135.0
171.90	943.0
172.90	1269.0
173.90	116800.0
174.90	8331.0
175.90	115680.0
176.90	7522.0
177.90	256.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278