


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092518\
 Data File : VV007847.D
 Acq On : 25 Sep 2018 10:53
 Operator : SY/MD
 Sample : BFB73
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB73

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM092518WMA.M
 Title : VOC Analysis
 Last Update : Wed Sep 26 04:58:06 2018

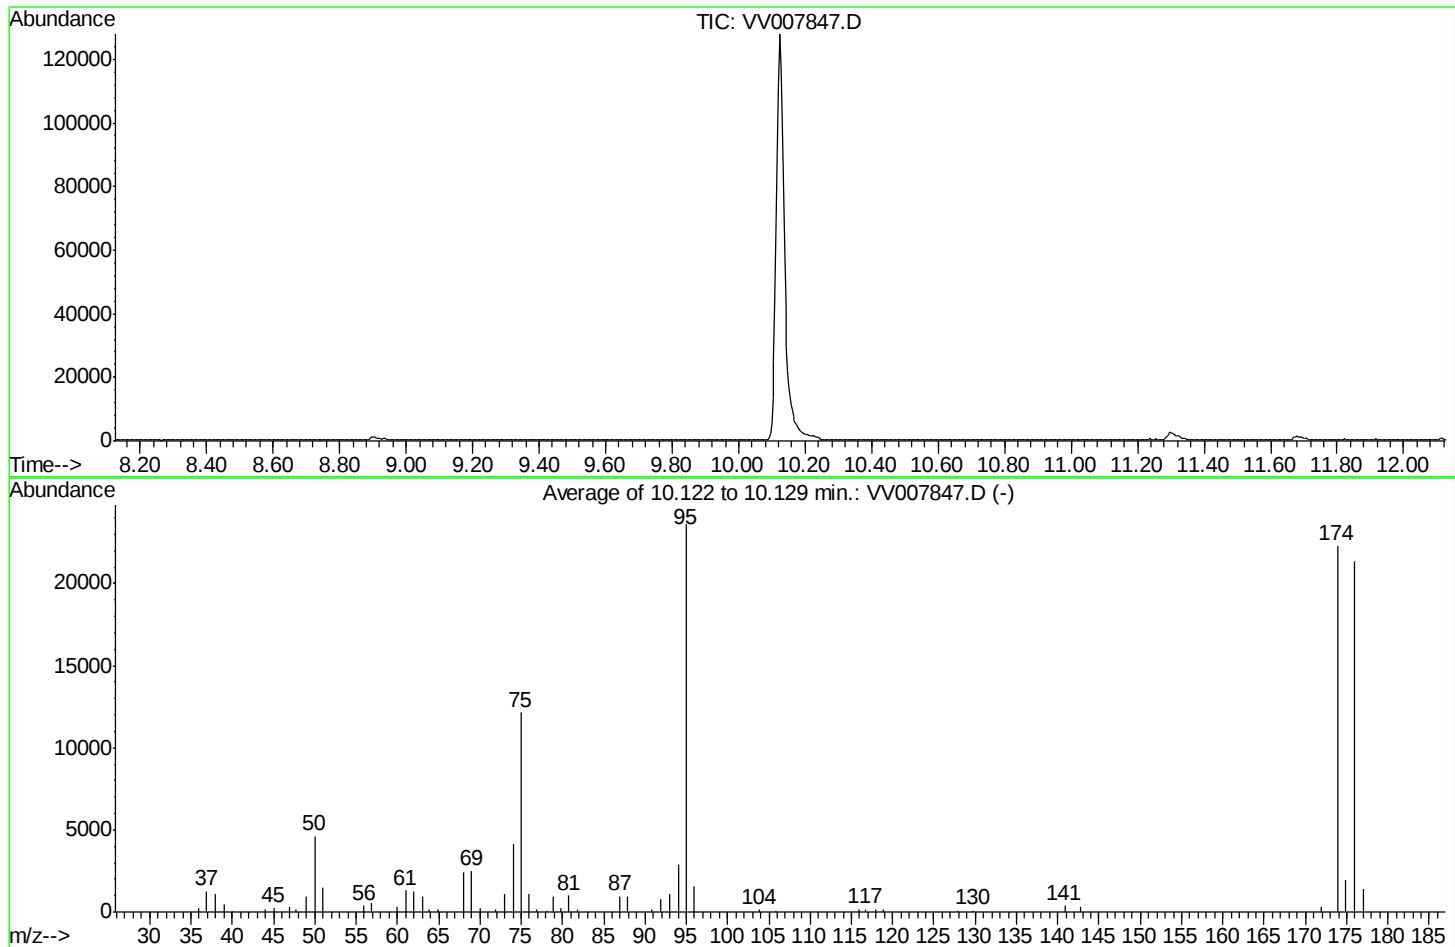

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	4604	PASS
75	95	30	80	51.5	12146	PASS
95	95	100	100	100.0	23602	PASS
96	95	5	9	6.6	1569	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	94.5	22312	PASS
175	174	5	9	8.7	1945	PASS
176	174	95	101	95.9	21389	PASS
177	176	5	9	6.4	1367	PASS

Scan 2798 (10.087 min): VV007847.D
BFB73

m/z	Abundance
39.90	102.0
44.00	326.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.90	246.0
36.90	1275.0
38.00	1179.0
39.00	563.0
40.00	134.0
43.90	486.0
45.00	242.0
46.90	397.0
47.70	148.0
48.90	986.0
50.00	4798.0
51.00	1558.0
56.00	377.0
56.90	608.0
59.90	305.0
61.00	1332.0
62.00	1251.0
63.00	1027.0
63.90	133.0
65.00	165.0
68.00	2507.0
69.00	2623.0
70.00	274.0
72.00	157.0
73.00	1166.0
74.00	4161.0
75.00	12722.0
76.00	1155.0
76.90	165.0
78.90	1004.0
79.90	274.0
80.80	951.0
81.90	191.0
86.90	859.0
87.90	954.0
90.70	133.0
91.90	778.0
93.00	1175.0
94.00	2950.0
95.00	24336.0
96.00	1592.0
103.90	137.0
105.90	122.0
115.90	135.0
116.80	208.0
117.90	128.0
118.90	165.0
129.70	112.0
140.90	398.0
142.80	343.0
171.90	290.0
173.90	22016.0
174.90	1880.0
175.90	21360.0
176.90	1448.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.90	240.0
36.90	1309.0
38.00	1162.0
39.00	509.0
39.90	152.0
43.90	457.0
45.00	256.0
46.90	376.0
47.80	145.0
48.90	940.0
50.00	4726.0
51.00	1519.0
55.90	358.0
56.90	591.0
59.90	307.0
61.00	1352.0
62.00	1279.0
63.00	1022.0
63.90	142.0
64.90	177.0
68.00	2434.0
69.00	2580.0
70.00	244.0
72.00	137.0
73.00	1146.0
74.00	4274.0
75.00	12597.0
76.00	1136.0
76.90	175.0
78.10	104.0
78.80	983.0
79.80	279.0
80.80	1034.0
81.80	177.0
86.90	997.0
87.80	905.0
90.70	128.0
91.90	818.0
92.90	1141.0
94.00	2945.0
95.00	24448.0
96.00	1618.0
103.80	135.0
105.80	121.0
115.90	138.0
116.80	194.0
117.90	147.0
118.90	153.0
127.80	112.0
129.80	122.0
140.80	380.0
142.80	361.0
171.90	311.0
173.90	23008.0
174.90	2032.0
175.90	22056.0
177.00	1383.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
36.00	243.0
36.90	1241.0
38.00	1013.0
38.90	443.0
39.90	135.0
44.00	432.0
45.00	259.0
46.90	280.0
47.80	141.0
48.90	783.0
50.00	4288.0
51.00	1326.0
55.90	344.0
56.90	552.0
60.00	273.0
61.00	1228.0
61.90	1188.0
63.00	862.0
63.90	153.0
64.90	200.0
68.00	2237.0
69.00	2333.0
70.00	200.0
71.90	113.0
73.00	1059.0
74.00	3981.0
75.00	11120.0
76.00	1066.0
76.90	134.0
78.00	114.0
78.80	910.0
79.80	272.0
80.80	998.0
81.80	170.0
87.00	979.0
87.80	893.0
90.80	125.0
91.90	788.0
92.90	1001.0
94.00	2673.0
95.00	22024.0
96.00	1497.0
103.80	109.0
105.70	107.0
115.90	116.0
116.70	179.0
118.00	130.0
118.90	136.0
127.80	133.0
129.80	116.0
140.90	305.0
142.80	354.0
171.90	288.0
173.90	21912.0
174.90	1924.0
175.90	20752.0
177.00	1270.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73