

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092520\
 Data File : VV018474.D
 Acq On : 25 Sep 2020 22:18
 Operator : SY/MD
 Sample : L4117-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	89	rVB	209040	209388	15.55%	1.883%
2	1.579	144	152	165	rBV	164013	184570	13.71%	1.660%
3	2.122	311	321	364	rVB	334062	522802	38.82%	4.702%
4	2.466	426	428	434	rVB2	323	152	0.01%	0.001%
5	2.531	441	448	453	rBV3	957	1426	0.11%	0.013%
6	2.788	519	528	537	rVB7	3613	6762	0.50%	0.061%
7	3.064	605	614	626	rBV6	2942	5848	0.43%	0.053%
8	3.267	674	677	684	rVB2	232	255	0.02%	0.002%
9	3.383	710	713	720	rVB	247	253	0.02%	0.002%
10	3.418	720	724	727	rBV	159	163	0.01%	0.001%
11	3.524	749	757	764	rBV2	114	161	0.01%	0.001%
12	3.804	839	844	849	rVB3	299	250	0.02%	0.002%
13	3.936	868	885	921	rBV2	172359	571909	42.47%	5.143%
14	4.376	1006	1022	1056	rBV	210620	518088	38.47%	4.659%
15	4.707	1122	1125	1129	rBV2	189	170	0.01%	0.002%
16	5.074	1220	1239	1266	rBV2	528258	1346600	100.00%	12.110%
17	5.415	1342	1345	1346	rBV2	226	147	0.01%	0.001%
18	5.453	1354	1357	1362	rVB	323	293	0.02%	0.003%
19	5.486	1365	1367	1373	rVB3	225	165	0.01%	0.001%
20	5.521	1373	1378	1382	rVB4	302	329	0.02%	0.003%
21	5.640	1402	1415	1443	rBV	432366	854376	63.45%	7.684%
22	5.939	1494	1508	1539	rBV3	171181	355409	26.39%	3.196%
23	6.093	1543	1556	1588	rVV	296619	596620	44.31%	5.366%
24	6.206	1588	1591	1593	rVB2	426	252	0.02%	0.002%
25	6.235	1596	1600	1602	rBV3	614	392	0.03%	0.004%
26	6.280	1613	1614	1619	rVB2	387	210	0.02%	0.002%
27	6.431	1655	1661	1667	rBV2	159	220	0.02%	0.002%
28	6.756	1756	1762	1765	rBV2	167	180	0.01%	0.002%
29	7.010	1829	1841	1868	rBV	166179	299960	22.28%	2.698%
30	7.167	1888	1890	1896	rVB3	227	177	0.01%	0.002%
31	7.241	1911	1913	1917	rVB2	274	211	0.02%	0.002%
32	7.338	1930	1943	1966	rBV	642812	1089615	80.92%	9.799%
33	7.585	2017	2020	2025	rVB2	311	284	0.02%	0.003%
34	7.643	2025	2038	2067	rBV	117526	205602	15.27%	1.849%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092520\
 Data File : VV018474.D
 Acq On : 25 Sep 2020 22:18
 Operator : SY/MD
 Sample : L4117-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	7.813	2089	2091	2093	rBV	244	158	0.01%	0.001%
36	7.955	2129	2135	2137	rBV3	579	618	0.05%	0.006%
37	8.109	2173	2183	2217	rBV2	292006	558961	41.51%	5.027%
38	8.312	2244	2246	2249	rVB3	538	321	0.02%	0.003%
39	8.331	2249	2252	2257	rVV4	419	384	0.03%	0.003%
40	8.367	2260	2263	2266	rVB	334	150	0.01%	0.001%
41	8.421	2275	2280	2285	rBV3	247	317	0.02%	0.003%
42	8.508	2304	2307	2310	rBV	209	164	0.01%	0.001%
43	8.569	2317	2326	2330	rBV2	226	328	0.02%	0.003%
44	8.875	2405	2421	2445	rBV	642227	1041131	77.32%	9.363%
45	9.039	2469	2472	2475	rBV4	271	180	0.01%	0.002%
46	9.174	2506	2514	2522	rVB3	761	1259	0.09%	0.011%
47	9.222	2526	2529	2534	rVB2	273	223	0.02%	0.002%
48	9.312	2554	2557	2563	rVB2	193	165	0.01%	0.001%
49	9.370	2571	2575	2580	rBV2	150	173	0.01%	0.002%
50	9.575	2634	2639	2642	rBV2	271	274	0.02%	0.002%
51	9.739	2685	2690	2695	rBV3	306	282	0.02%	0.003%
52	10.035	2776	2782	2786	rBV2	325	325	0.02%	0.003%
53	10.080	2792	2796	2798	rBV	265	184	0.01%	0.002%
54	10.141	2810	2815	2816	rBV3	821	675	0.05%	0.006%
55	10.238	2832	2845	2866	rBV	380519	589623	43.79%	5.303%
56	10.383	2880	2890	2892	rBV5	797	997	0.07%	0.009%
57	10.399	2892	2895	2907	rVB2	1165	1617	0.12%	0.015%
58	10.473	2911	2918	2925	rBV5	2162	3714	0.28%	0.033%
59	10.559	2941	2945	2950	rBV3	887	1022	0.08%	0.009%
60	10.601	2950	2958	2968	rVB3	6045	9444	0.70%	0.085%
61	10.720	2988	2995	3000	rBV2	424	476	0.04%	0.004%
62	10.759	3001	3007	3008	rBV2	317	288	0.02%	0.003%
63	10.855	3030	3037	3040	rBV3	571	687	0.05%	0.006%
64	10.900	3045	3051	3056	rVV3	1976	2415	0.18%	0.022%
65	10.939	3057	3063	3073	rVV2	4610	6649	0.49%	0.060%
66	10.981	3073	3076	3082	rVB4	803	719	0.05%	0.006%
67	11.032	3087	3092	3094	rBV	228	193	0.01%	0.002%
68	11.055	3094	3099	3105	rVB2	547	627	0.05%	0.006%
69	11.119	3114	3119	3124	rBV3	484	505	0.04%	0.005%
70	11.170	3129	3135	3142	rBV5	835	1039	0.08%	0.009%
71	11.270	3151	3166	3189	rBV	682705	1041249	77.32%	9.364%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092520\
 Data File : VV018474.D
 Acq On : 25 Sep 2020 22:18
 Operator : SY/MD
 Sample : L4117-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

72	11.357	3189	3193	3200	rVV6	2736	4260	0.32%	0.038%
73	11.392	3200	3204	3218	rVV7	3075	5641	0.42%	0.051%
74	11.450	3218	3222	3225	rVV5	976	994	0.07%	0.009%
75	11.485	3227	3233	3240	rVB4	1879	2655	0.20%	0.024%
76	11.563	3252	3257	3258	rBV2	356	253	0.02%	0.002%
77	11.646	3270	3283	3312	rBV	643792	1019258	75.69%	9.166%
78	11.810	3325	3334	3352	rVV2	15388	22655	1.68%	0.204%
79	11.881	3354	3356	3360	rVB	393	194	0.01%	0.002%
80	11.939	3370	3374	3376	rBV	476	401	0.03%	0.004%
81	11.955	3376	3379	3381	rVV2	313	247	0.02%	0.002%
82	12.013	3388	3397	3407	rBV6	1363	2512	0.19%	0.023%
83	12.087	3418	3420	3427	rVB3	540	508	0.04%	0.005%
84	12.135	3430	3435	3438	rBV4	735	723	0.05%	0.007%
85	12.273	3472	3478	3483	rBV3	548	613	0.05%	0.006%
86	12.389	3505	3514	3520	rBV4	1869	2712	0.20%	0.024%
87	12.424	3520	3525	3526	rBV4	607	504	0.04%	0.005%
88	12.492	3536	3546	3549	rBV5	1024	1249	0.09%	0.011%
89	12.527	3552	3557	3563	rVB4	1020	1136	0.08%	0.010%
90	12.611	3579	3583	3588	rVB3	720	697	0.05%	0.006%
91	12.675	3598	3603	3605	rBV	227	193	0.01%	0.002%
92	12.910	3669	3676	3685	rBV3	4925	6603	0.49%	0.059%
93	13.064	3717	3724	3734	rVB6	861	1355	0.10%	0.012%
94	13.501	3857	3860	3865	rVB2	416	370	0.03%	0.003%
95	13.546	3866	3874	3877	rBV4	495	642	0.05%	0.006%
96	13.659	3906	3909	3911	rBV2	483	333	0.02%	0.003%
97	13.746	3933	3936	3938	rBV2	217	163	0.01%	0.001%
98	13.836	3962	3964	3973	rVB3	198	273	0.02%	0.002%
99	13.874	3973	3976	3979	rBV	268	202	0.02%	0.002%
100	13.926	3986	3992	3998	rVB4	1105	1260	0.09%	0.011%


Sum of corrected areas: 11119381

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092520\
Data File : VV018474.D
Acq On : 25 Sep 2020 22:18
Operator : SY/MD
Sample : L4117-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
E0AA8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

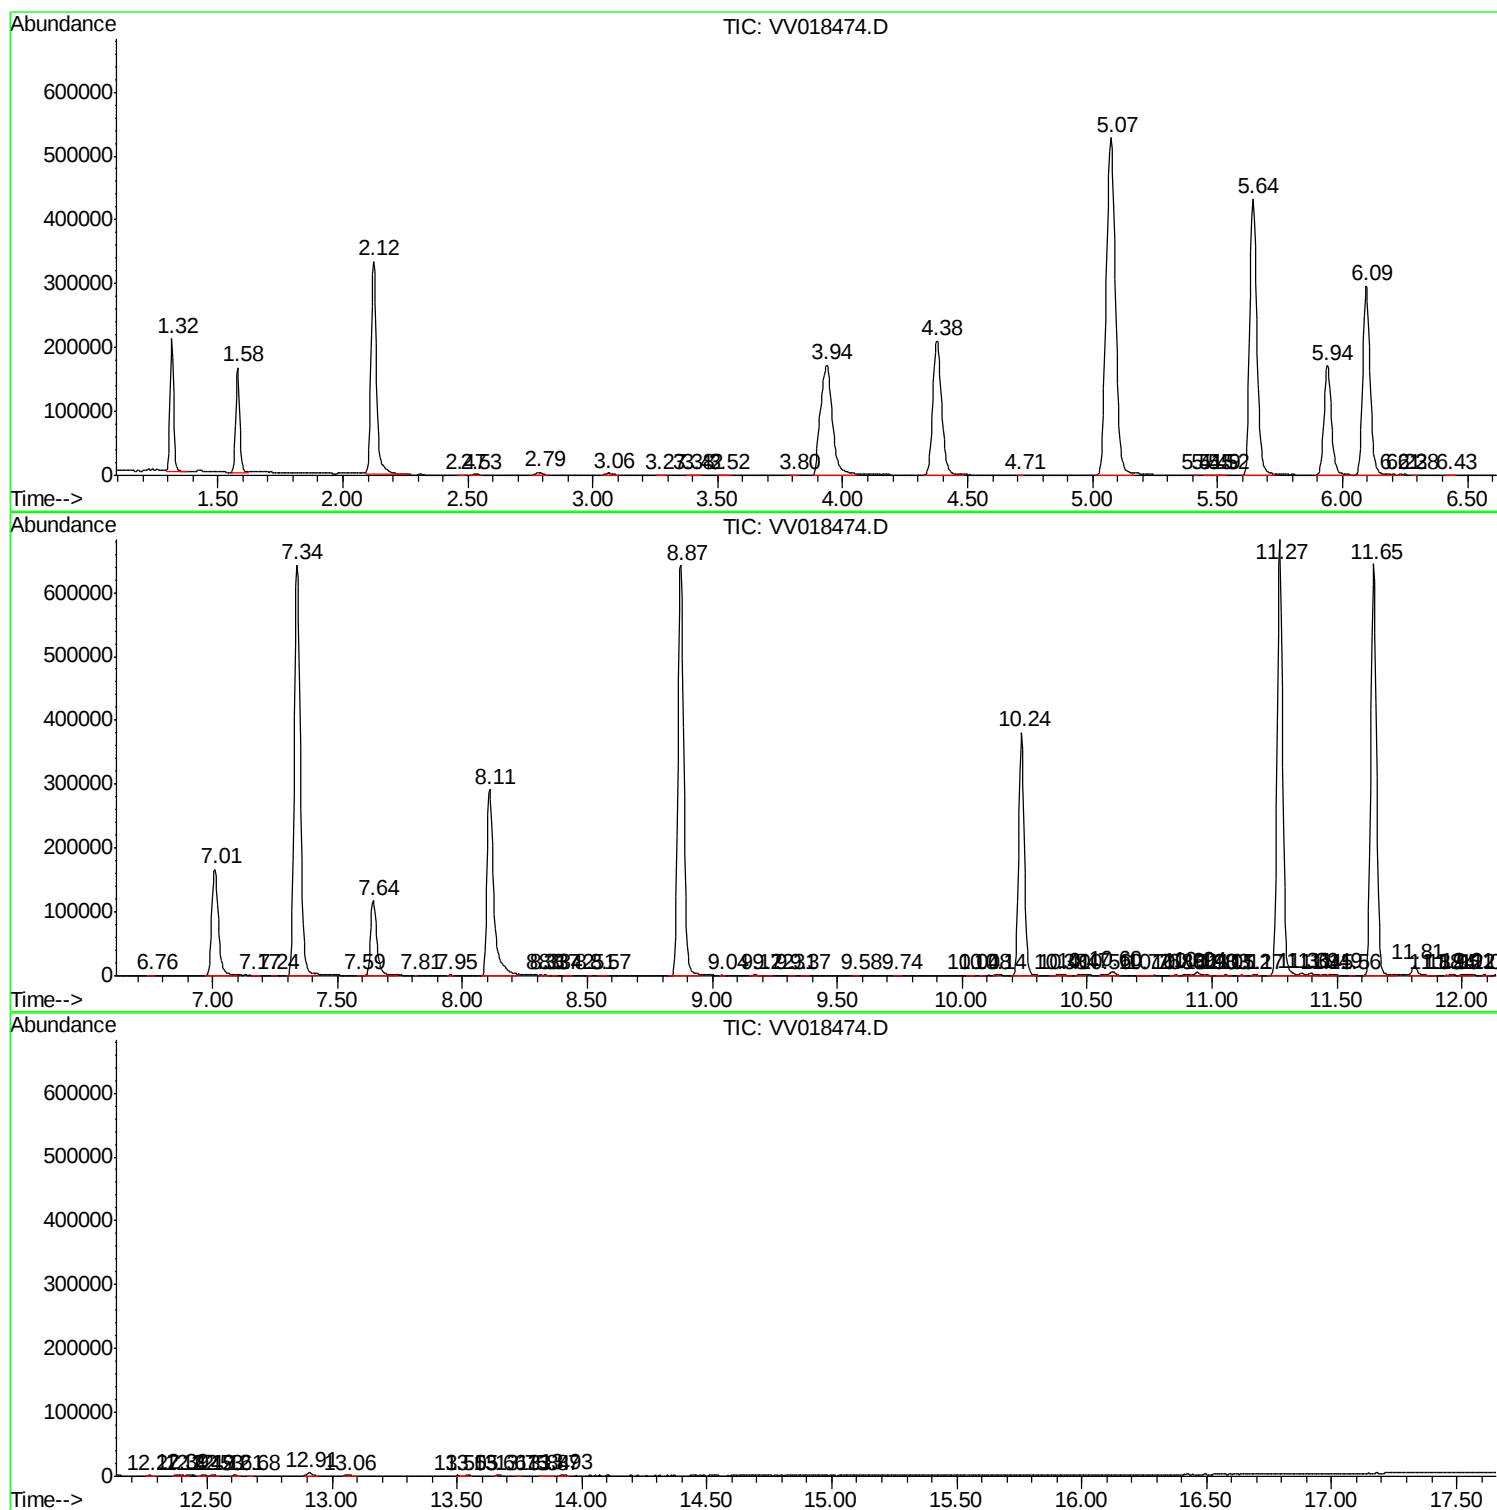

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV092520\
Data File : VV018474.D
Acq On : 25 Sep 2020 22:18
Operator : SY/MD
Sample : L4117-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV092520\
Data File : VV018474.D
Acq On : 25 Sep 2020 22:18
Operator : SY/MD
Sample : L4117-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA8

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc