

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092520\
 Data File : VV018475.D
 Acq On : 25 Sep 2020 22:40
 Operator : SY/MD
 Sample : L4117-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	88	rVB	202281	199263	7.38%	1.504%
2	1.579	144	152	167	rBV	159578	184392	6.83%	1.392%
3	2.123	310	321	348	rVB	325861	495598	18.37%	3.741%
4	2.531	441	448	449	rBV	931	873	0.03%	0.007%
5	2.605	465	471	473	rBV	154	158	0.01%	0.001%
6	2.653	482	486	489	rBV2	164	167	0.01%	0.001%
7	2.785	518	527	542	rVB3	5906	11138	0.41%	0.084%
8	3.068	603	615	627	rBV5	2774	5538	0.21%	0.042%
9	3.225	657	664	669	rBV2	156	207	0.01%	0.002%
10	3.303	684	688	693	rBV2	153	152	0.01%	0.001%
11	3.521	753	756	762	rVB	220	164	0.01%	0.001%
12	3.679	802	805	810	rVB2	171	154	0.01%	0.001%
13	3.711	810	815	819	rBV2	155	173	0.01%	0.001%
14	3.936	868	885	920	rBV3	173334	561393	20.80%	4.238%
15	4.376	1005	1022	1050	rBV	208108	510956	18.93%	3.857%
16	4.991	1211	1213	1217	rVB2	215	154	0.01%	0.001%
17	5.074	1221	1239	1275	rBV2	524588	1331544	49.34%	10.051%
18	5.338	1317	1321	1325	rBV3	202	147	0.01%	0.001%
19	5.412	1340	1344	1348	rVB2	242	206	0.01%	0.002%
20	5.438	1348	1352	1355	rBV2	392	355	0.01%	0.003%
21	5.499	1368	1371	1375	rVV2	201	232	0.01%	0.002%
22	5.589	1396	1399	1403	rVB2	195	150	0.01%	0.001%
23	5.640	1403	1415	1441	rBV	415501	824975	30.57%	6.227%
24	5.859	1480	1483	1488	rBV2	240	191	0.01%	0.001%
25	5.936	1493	1507	1540	rBV	1385913	2698510	100.00%	20.369%
26	6.093	1543	1556	1583	rVB	295187	593295	21.99%	4.478%
27	6.319	1624	1626	1630	rVV2	284	209	0.01%	0.002%
28	6.347	1633	1635	1640	rVB2	234	157	0.01%	0.001%
29	6.412	1648	1655	1657	rBV2	208	176	0.01%	0.001%
30	6.511	1682	1686	1690	rBV	197	176	0.01%	0.001%
31	6.611	1713	1717	1720	rBV2	152	158	0.01%	0.001%
32	7.010	1829	1841	1868	rBV	164287	295115	10.94%	2.228%
33	7.148	1880	1884	1891	rVB4	512	491	0.02%	0.004%
34	7.338	1930	1943	1982	rBV	622704	1077161	39.92%	8.131%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092520\
 Data File : VV018475.D
 Acq On : 25 Sep 2020 22:40
 Operator : SY/MD
 Sample : L4117-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	7.643	2027	2038	2062	rBV	115479	200121	7.42%	1.511%
36	7.865	2105	2107	2111	rVV3	340	207	0.01%	0.002%
37	7.955	2130	2135	2145	rBV2	479	829	0.03%	0.006%
38	8.042	2157	2162	2167	rBV2	194	239	0.01%	0.002%
39	8.109	2172	2183	2226	rBV	287216	546844	20.26%	4.128%
40	8.498	2301	2304	2310	rBV3	302	217	0.01%	0.002%
41	8.543	2315	2318	2322	rVB	190	148	0.01%	0.001%
42	8.707	2365	2369	2373	rVB2	173	152	0.01%	0.001%
43	8.875	2409	2421	2457	rBV	626175	1016127	37.66%	7.670%
44	9.039	2469	2472	2474	rBV3	275	203	0.01%	0.002%
45	9.109	2489	2494	2499	rVV3	293	317	0.01%	0.002%
46	9.161	2505	2510	2511	rBV2	559	362	0.01%	0.003%
47	9.228	2529	2531	2538	rBV4	281	297	0.01%	0.002%
48	9.566	2634	2636	2638	rBV2	214	149	0.01%	0.001%
49	9.733	2685	2688	2691	rBV	271	171	0.01%	0.001%
50	9.955	2754	2757	2761	rVB	266	237	0.01%	0.002%
51	10.035	2779	2782	2784	rBV3	272	156	0.01%	0.001%
52	10.084	2793	2797	2799	rBV	219	175	0.01%	0.001%
53	10.113	2804	2806	2810	rVV3	316	230	0.01%	0.002%
54	10.142	2810	2815	2823	rVB6	1199	1827	0.07%	0.014%
55	10.238	2832	2845	2863	rBV	372930	577714	21.41%	4.361%
56	10.367	2882	2885	2887	rBV2	302	197	0.01%	0.001%
57	10.396	2888	2894	2906	rVB4	1032	1852	0.07%	0.014%
58	10.473	2906	2918	2924	rBV3	2476	3999	0.15%	0.030%
59	10.566	2940	2947	2950	rBV3	1423	1514	0.06%	0.011%
60	10.601	2950	2958	2971	rVB2	5755	8954	0.33%	0.068%
61	10.717	2990	2994	3001	rBV3	399	452	0.02%	0.003%
62	10.762	3002	3008	3012	rVV2	576	710	0.03%	0.005%
63	10.794	3016	3018	3024	rVB3	364	298	0.01%	0.002%
64	10.826	3024	3028	3032	rBV3	173	156	0.01%	0.001%
65	10.862	3032	3039	3043	rVB2	538	649	0.02%	0.005%
66	10.897	3043	3050	3056	rBV3	2150	2864	0.11%	0.022%
67	10.942	3056	3064	3076	rBV2	4191	6237	0.23%	0.047%
68	11.055	3093	3099	3106	rBV4	860	781	0.03%	0.006%
69	11.087	3106	3109	3115	rVB3	298	277	0.01%	0.002%
70	11.122	3115	3120	3124	rBV3	479	472	0.02%	0.004%
71	11.174	3129	3136	3139	rBV4	990	1306	0.05%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092520\
 Data File : VV018475.D
 Acq On : 25 Sep 2020 22:40
 Operator : SY/MD
 Sample : L4117-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AA9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

72	11.270	3154	3166	3188	rVV	665865	1014834	37.61%	7.660%
73	11.354	3188	3192	3200	rVV5	3085	5176	0.19%	0.039%
74	11.395	3201	3205	3215	rVV6	3179	4673	0.17%	0.035%
75	11.444	3215	3220	3226	rVV2	758	858	0.03%	0.006%
76	11.489	3226	3234	3243	rVB4	1766	2691	0.10%	0.020%
77	11.646	3270	3283	3305	rBV	648921	1006753	37.31%	7.599%
78	11.810	3323	3334	3343	rBV	13673	20363	0.75%	0.154%
79	11.932	3368	3372	3375	rBV2	271	209	0.01%	0.002%
80	11.961	3375	3381	3386	rVB5	675	819	0.03%	0.006%
81	12.013	3389	3397	3399	rBV4	1148	1319	0.05%	0.010%
82	12.093	3417	3422	3426	rVB3	462	353	0.01%	0.003%
83	12.145	3432	3438	3443	rVB5	853	1103	0.04%	0.008%
84	12.209	3456	3458	3461	rVB	274	154	0.01%	0.001%
85	12.273	3476	3478	3488	rVB3	344	278	0.01%	0.002%
86	12.379	3504	3511	3513	rBV5	1851	1923	0.07%	0.015%
87	12.489	3538	3545	3550	rBV5	1121	1265	0.05%	0.010%
88	12.527	3550	3557	3563	rVV4	1045	1452	0.05%	0.011%
89	12.614	3578	3584	3593	rVB4	1093	1307	0.05%	0.010%
90	12.659	3593	3598	3600	rBV2	258	225	0.01%	0.002%
91	12.698	3606	3610	3615	rBV2	179	221	0.01%	0.002%
92	12.910	3668	3676	3685	rVB4	4430	6317	0.23%	0.048%
93	13.064	3718	3724	3732	rVB5	948	1281	0.05%	0.010%
94	13.219	3769	3772	3781	rVB	250	237	0.01%	0.002%
95	13.498	3857	3859	3867	rVB3	329	210	0.01%	0.002%
96	13.543	3871	3873	3879	rVB	311	254	0.01%	0.002%
97	13.714	3923	3926	3928	rBV	240	163	0.01%	0.001%
98	13.926	3985	3992	3996	rBV3	1227	1574	0.06%	0.012%
99	14.077	4036	4039	4044	rBV2	351	404	0.01%	0.003%
100	15.569	4501	4503	4509	rVB2	645	436	0.02%	0.003%


Sum of corrected areas: 13248020

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092520\
Data File : VV018475.D
Acq On : 25 Sep 2020 22:40
Operator : SY/MD
Sample : L4117-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

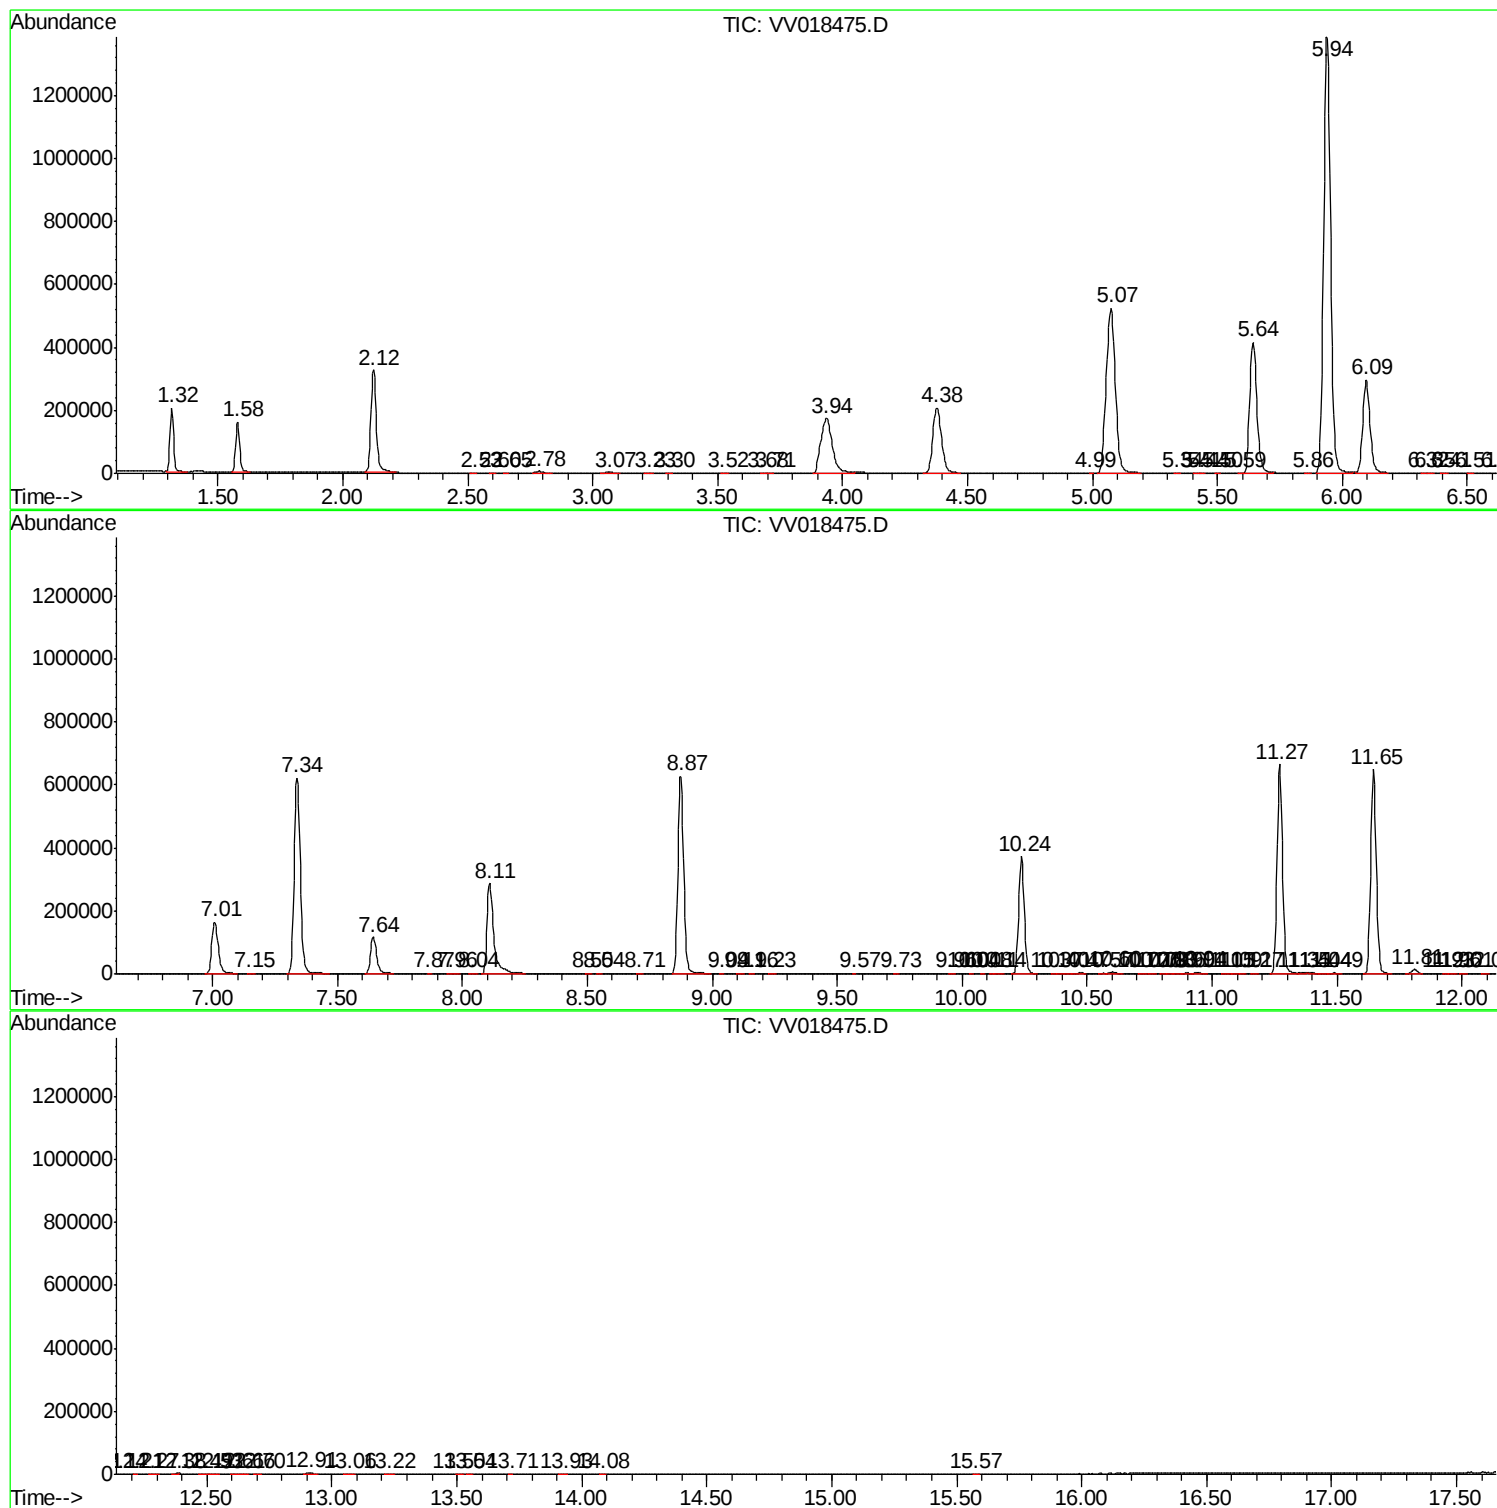

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV092520\
Data File : VV018475.D
Acq On : 25 Sep 2020 22:40
Operator : SY/MD
Sample : L4117-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV092520\
Data File : VV018475.D
Acq On : 25 Sep 2020 22:40
Operator : SY/MD
Sample : L4117-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AA9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc