

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092520\
 Data File : VV018477.D
 Acq On : 25 Sep 2020 23:26
 Operator : SY/MD
 Sample : L4117-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	82	rVB	199441	199741	14.92%	1.981%
2	1.579	144	152	166	rBV	165697	187426	14.00%	1.859%
3	2.122	311	321	355	rVB	321146	498026	37.21%	4.940%
4	2.772	519	523	524	rBV2	670	510	0.04%	0.005%
5	3.068	603	615	625	rBV5	2727	5234	0.39%	0.052%
6	3.184	646	651	653	rBV	179	166	0.01%	0.002%
7	3.785	835	838	843	rVB2	265	176	0.01%	0.002%
8	3.920	865	880	915	rBV	86683	278184	20.78%	2.760%
9	4.376	1005	1022	1059	rBV	212500	519912	38.84%	5.158%
10	4.634	1100	1102	1105	rVV2	268	179	0.01%	0.002%
11	4.669	1108	1113	1116	rBV2	335	280	0.02%	0.003%
12	4.740	1133	1135	1140	rVB2	285	193	0.01%	0.002%
13	4.765	1140	1143	1146	rBV	297	182	0.01%	0.002%
14	4.814	1153	1158	1160	rBV2	258	228	0.02%	0.002%
15	4.859	1169	1172	1176	rBV2	254	180	0.01%	0.002%
16	5.074	1220	1239	1272	rBV2	527673	1338462	100.00%	13.278%
17	5.312	1310	1313	1317	rVB3	257	193	0.01%	0.002%
18	5.396	1336	1339	1343	rVB	179	155	0.01%	0.002%
19	5.421	1343	1347	1351	rBV2	201	198	0.01%	0.002%
20	5.457	1356	1358	1362	rVB	278	184	0.01%	0.002%
21	5.643	1402	1416	1446	rBV	407466	809415	60.47%	8.030%
22	5.933	1494	1506	1529	rVB3	21139	48583	3.63%	0.482%
23	6.093	1542	1556	1586	rBV	295189	599182	44.77%	5.944%
24	6.289	1612	1617	1623	rBV2	386	341	0.03%	0.003%
25	6.418	1650	1657	1662	rBV2	161	270	0.02%	0.003%
26	6.798	1770	1775	1781	rVB2	229	300	0.02%	0.003%
27	7.010	1825	1841	1867	rBV	162568	292564	21.86%	2.902%
28	7.338	1931	1943	1968	rBV	618156	1058811	79.11%	10.504%
29	7.643	2027	2038	2072	rBV	114778	201126	15.03%	1.995%
30	7.897	2113	2117	2119	rBV	249	189	0.01%	0.002%
31	7.910	2119	2121	2128	rVB	234	209	0.02%	0.002%
32	7.945	2128	2132	2133	rBV	477	260	0.02%	0.003%
33	7.958	2134	2136	2152	rVB2	664	910	0.07%	0.009%
34	8.109	2173	2183	2229	rBV	297711	566074	42.29%	5.616%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092520\
 Data File : VV018477.D
 Acq On : 25 Sep 2020 23:26
 Operator : SY/MD
 Sample : L4117-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

35	8.325	2248	2250	2253	rVB3	252	166	0.01%	0.002%
36	8.383	2265	2268	2273	rVB2	233	209	0.02%	0.002%
37	8.437	2281	2285	2292	rBV2	164	247	0.02%	0.002%
38	8.511	2305	2308	2314	rVB2	243	164	0.01%	0.002%
39	8.543	2314	2318	2321	rBV2	229	211	0.02%	0.002%
40	8.566	2321	2325	2330	rVB3	239	214	0.02%	0.002%
41	8.875	2409	2421	2454	rBV	599403	971433	72.58%	9.637%
42	9.170	2506	2513	2519	rBV4	847	1155	0.09%	0.011%
43	9.231	2530	2532	2541	rVB3	365	370	0.03%	0.004%
44	9.280	2541	2547	2552	rBV2	134	183	0.01%	0.002%
45	9.502	2608	2616	2619	rBV2	130	172	0.01%	0.002%
46	9.569	2633	2637	2645	rBV3	536	706	0.05%	0.007%
47	9.617	2648	2652	2658	rVB	148	155	0.01%	0.002%
48	9.678	2666	2671	2676	rBV	191	205	0.02%	0.002%
49	9.839	2717	2721	2725	rVB	234	208	0.02%	0.002%
50	9.958	2754	2758	2763	rVB2	257	266	0.02%	0.003%
51	10.103	2801	2803	2809	rBV3	346	403	0.03%	0.004%
52	10.148	2809	2817	2822	rVB4	1253	1751	0.13%	0.017%
53	10.238	2832	2845	2865	rBV	375119	581898	43.48%	5.773%
54	10.373	2882	2887	2889	rBV2	496	389	0.03%	0.004%
55	10.476	2912	2919	2924	rBV3	1845	2665	0.20%	0.026%
56	10.566	2939	2947	2951	rVV	1046	1457	0.11%	0.014%
57	10.601	2951	2958	2968	rVB2	5290	7919	0.59%	0.079%
58	10.649	2968	2973	2976	rBV2	151	167	0.01%	0.002%
59	10.717	2991	2994	2998	rBV2	328	265	0.02%	0.003%
60	10.759	3003	3007	3008	rBV	460	317	0.02%	0.003%
61	10.855	3029	3037	3044	rBV3	554	788	0.06%	0.008%
62	10.900	3044	3051	3056	rBV4	1483	2185	0.16%	0.022%
63	10.939	3056	3063	3074	rVB2	3689	5199	0.39%	0.052%
64	11.055	3094	3099	3107	rVB4	682	794	0.06%	0.008%
65	11.122	3117	3120	3126	rVB2	247	207	0.02%	0.002%
66	11.174	3129	3136	3142	rVB5	876	1094	0.08%	0.011%
67	11.212	3143	3148	3153	rVB2	219	256	0.02%	0.003%
68	11.270	3154	3166	3186	rBV	594166	907132	67.77%	8.999%
69	11.395	3200	3205	3215	rVB5	2861	4365	0.33%	0.043%
70	11.450	3215	3222	3227	rBV4	651	923	0.07%	0.009%
71	11.485	3227	3233	3241	rVB6	1792	2309	0.17%	0.023%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV092520\
 Data File : VV018477.D
 Acq On : 25 Sep 2020 23:26
 Operator : SY/MD
 Sample : L4117-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
 Title : VOC Analysis

72	11.563	3251	3257	3259	rBV3	826	684	0.05%	0.007%
73	11.604	3266	3270	3271	rBV2	277	165	0.01%	0.002%
74	11.646	3271	3283	3302	rVV	601023	936385	69.96%	9.289%
75	11.810	3324	3334	3344	rBV	12477	18156	1.36%	0.180%
76	11.932	3368	3372	3375	rBV4	389	228	0.02%	0.002%
77	11.952	3375	3378	3379	rBV2	341	183	0.01%	0.002%
78	11.964	3379	3382	3386	rVB3	586	527	0.04%	0.005%
79	12.010	3389	3396	3401	rBV4	1093	1494	0.11%	0.015%
80	12.093	3417	3422	3427	rBV4	497	418	0.03%	0.004%
81	12.145	3433	3438	3439	rBV2	660	497	0.04%	0.005%
82	12.196	3450	3454	3460	rBV2	160	201	0.02%	0.002%
83	12.276	3471	3479	3484	rVB2	429	582	0.04%	0.006%
84	12.325	3491	3494	3497	rBV	262	186	0.01%	0.002%
85	12.389	3507	3514	3520	rBV5	1287	1670	0.12%	0.017%
86	12.418	3520	3523	3525	rVV2	515	357	0.03%	0.004%
87	12.440	3528	3530	3534	rVV3	890	665	0.05%	0.007%
88	12.482	3538	3543	3548	rVV3	1116	919	0.07%	0.009%
89	12.527	3551	3557	3564	rVB3	685	763	0.06%	0.008%
90	12.611	3580	3583	3588	rVV3	631	677	0.05%	0.007%
91	12.813	3643	3646	3650	rVB2	209	160	0.01%	0.002%
92	12.907	3669	3675	3686	rVB5	3863	5384	0.40%	0.053%
93	13.061	3719	3723	3730	rBV3	773	912	0.07%	0.009%
94	13.354	3811	3814	3818	rBV2	276	230	0.02%	0.002%
95	13.492	3853	3857	3859	rBV2	193	159	0.01%	0.002%
96	13.543	3868	3873	3876	rBV3	295	289	0.02%	0.003%
97	13.694	3917	3920	3922	rBV	317	236	0.02%	0.002%
98	13.823	3957	3960	3962	rBV2	304	204	0.02%	0.002%
99	13.894	3977	3982	3986	rBV3	280	298	0.02%	0.003%
100	13.926	3986	3992	3998	rVB3	1120	1269	0.09%	0.013%


Sum of corrected areas: 10080488

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV092520\
Data File : VV018477.D
Acq On : 25 Sep 2020 23:26
Operator : SY/MD
Sample : L4117-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
E0AB1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

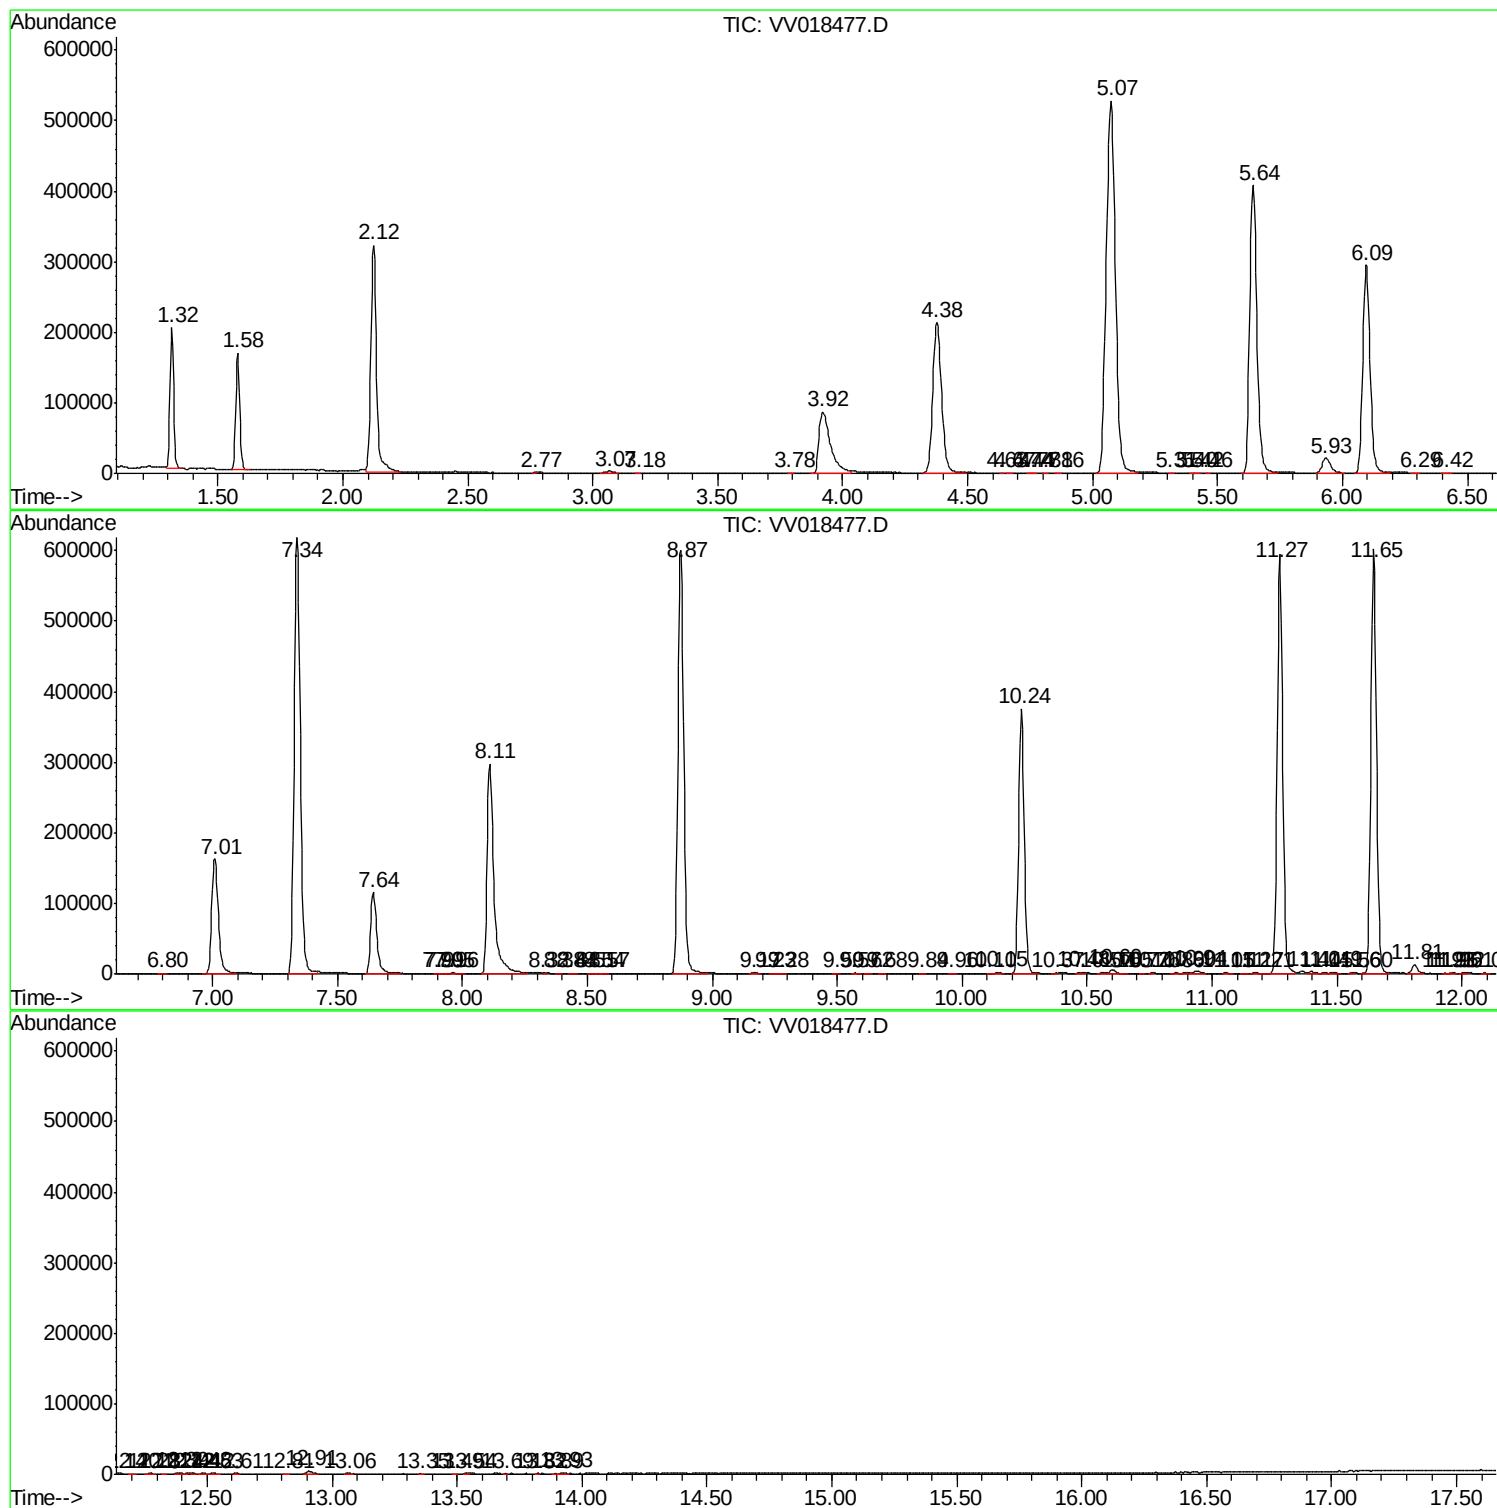

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV092520\
Data File : VV018477.D
Acq On : 25 Sep 2020 23:26
Operator : SY/MD
Sample : L4117-10
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
E0AB1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV092520\
Data File : VV018477.D
Acq On : 25 Sep 2020 23:26
Operator : SY/MD
Sample : L4117-10
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
E0AB1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc