


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV092520\
Data File : VV018440.D
Acq On : 25 Sep 2020 08:40
Operator : SY/MD
Sample : BFB99
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB99

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090920WMA.M
Title : VOC Analysis
Last Update : Mon Sep 28 03:12:36 2020

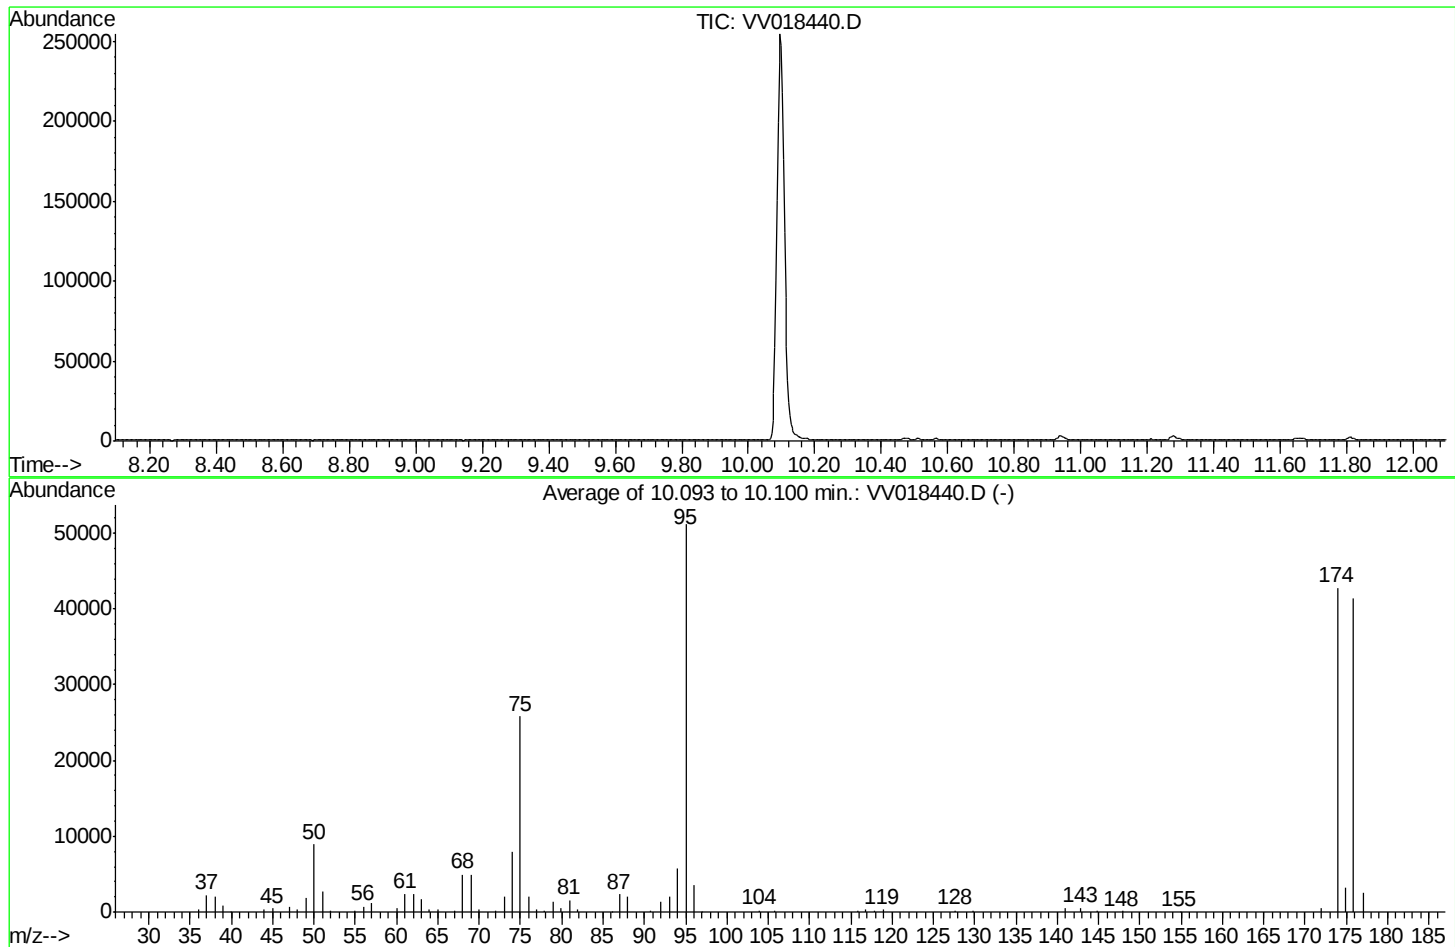

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	8953	PASS
75	95	30	80	50.5	25818	PASS
95	95	100	100	100.0	51157	PASS
96	95	5	9	7.0	3565	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.6	42768	PASS
175	174	5	9	7.5	3220	PASS
176	174	95	101	96.7	41357	PASS
177	176	5	9	6.2	2581	PASS

m/z	Abundance
40.00	238.0
43.90	350.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
36.00	420.0
37.00	2244.0
38.00	1985.0
39.00	887.0
39.90	267.0
44.00	635.0
45.00	436.0
47.00	597.0
48.00	339.0
49.00	1904.0
50.00	8645.0
51.00	2650.0
52.00	146.0
54.90	119.0
56.00	649.0
57.00	1173.0
60.00	491.0
61.00	2375.0
62.00	2294.0
63.00	1652.0
64.00	280.0
64.90	378.0
67.10	116.0
68.00	4696.0
69.00	4793.0
70.00	387.0
72.00	244.0
73.00	2008.0
74.00	7680.0
75.00	25224.0
76.00	2119.0
76.90	300.0
77.90	220.0
79.00	1314.0
79.90	467.0
80.90	1402.0
81.90	354.0
87.00	2245.0
88.00	2103.0
90.80	136.0
92.00	1376.0
93.00	1991.0
94.00	5530.0
95.00	49656.0
96.00	3495.0
97.00	118.0
104.00	185.0
105.80	164.0
115.90	167.0
116.80	289.0
117.90	151.0
118.90	296.0
127.70	183.0
129.80	169.0
140.90	461.0
142.90	496.0
144.80	162.0
147.90	158.0
171.90	500.0
173.90	40568.0
174.90	3012.0
175.90	38792.0
177.00	2435.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
36.00	402.0
37.00	2277.0
38.00	2086.0
39.00	915.0
39.90	239.0
44.00	639.0
45.00	468.0
47.00	618.0
48.00	344.0
49.00	1984.0
50.00	9293.0
51.00	2856.0
52.00	132.0
54.90	142.0
56.00	712.0
57.00	1231.0
60.00	466.0
61.00	2464.0
62.00	2357.0
63.00	1778.0
63.90	278.0
65.00	374.0
66.90	125.0
68.00	5176.0
69.00	5047.0
70.00	425.0
72.00	227.0
73.00	2195.0
74.00	8166.0
75.00	26704.0
76.00	2167.0
76.90	338.0
77.80	228.0
78.90	1437.0
79.90	496.0
80.90	1594.0
81.90	360.0
86.10	102.0
87.00	2373.0
88.00	2191.0
90.80	185.0
92.00	1464.0
93.00	2083.0
94.00	5992.0
95.00	52888.0
96.00	3706.0
97.00	102.0
104.00	212.0
105.80	170.0
115.80	180.0
116.90	284.0
117.90	183.0
118.90	321.0
127.70	237.0
129.80	180.0
140.90	503.0
142.80	567.0
144.80	148.0
147.90	155.0
154.90	103.0
171.90	560.0
173.90	44176.0
174.90	3314.0
175.90	42712.0
177.00	2625.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99

m/z	Abundance
35.90	382.0
37.00	2094.0
38.00	1949.0
39.00	877.0
39.90	225.0
44.00	611.0
45.00	474.0
47.00	580.0
48.00	285.0
49.00	1882.0
50.00	8921.0
51.00	2826.0
52.00	120.0
54.90	165.0
56.00	676.0
57.00	1183.0
60.00	386.0
61.00	2282.0
62.00	2235.0
63.00	1752.0
63.90	268.0
65.00	375.0
66.90	123.0
68.00	4988.0
69.00	4927.0
70.00	436.0
71.90	199.0
73.00	2082.0
74.00	7835.0
75.00	25528.0
76.00	1984.0
76.90	316.0
77.80	226.0
78.90	1413.0
79.90	456.0
80.90	1575.0
81.90	317.0
87.00	2241.0
88.00	2007.0
90.80	195.0
92.00	1445.0
93.00	2020.0
94.00	5842.0
95.00	50928.0
96.00	3494.0
103.90	231.0
105.80	163.0
115.80	186.0
116.90	278.0
117.90	202.0
118.90	293.0
127.70	255.0
129.90	187.0
140.90	471.0
142.80	590.0
144.80	129.0
147.90	116.0
154.90	117.0
171.90	532.0
173.90	43560.0
174.90	3334.0
175.90	42568.0
177.00	2685.0

Instrument :
MSVOA_V
ClientSampleId :
BFB99