
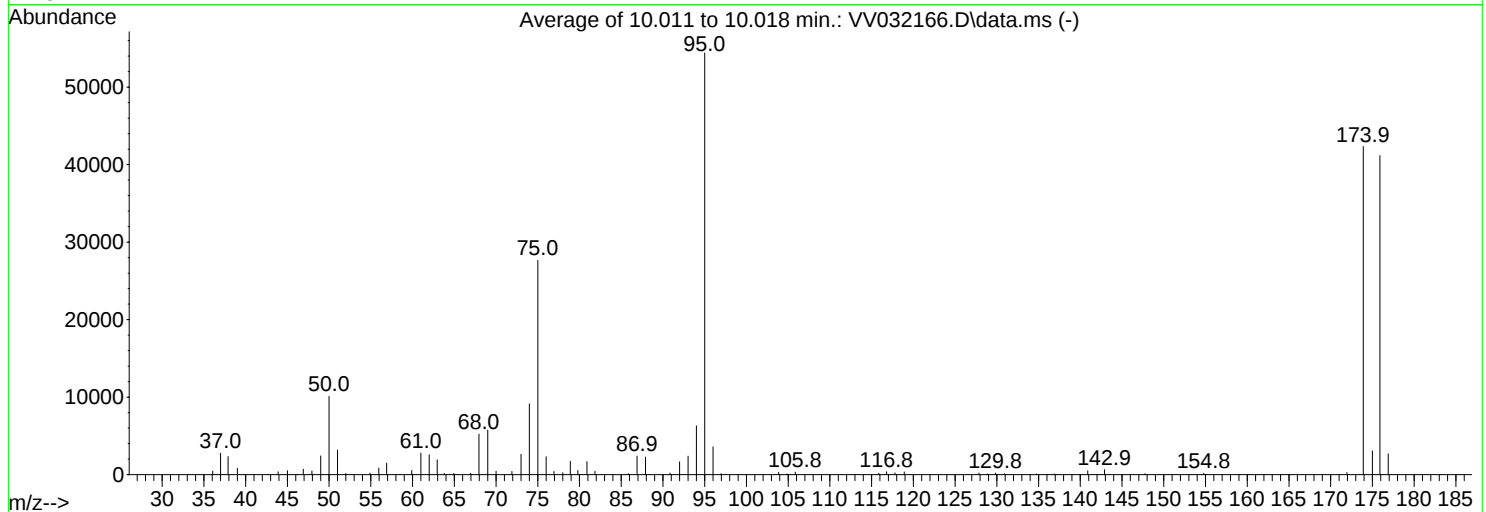


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092523\
Data File : VV032166.D
Acq On : 25 Sep 2023 11:02
Operator : SY/MD
Sample : BFB216
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB216

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092523WMA.M
Title : VOC Analysis
Last Update : Tue Sep 26 01:18:56 2023

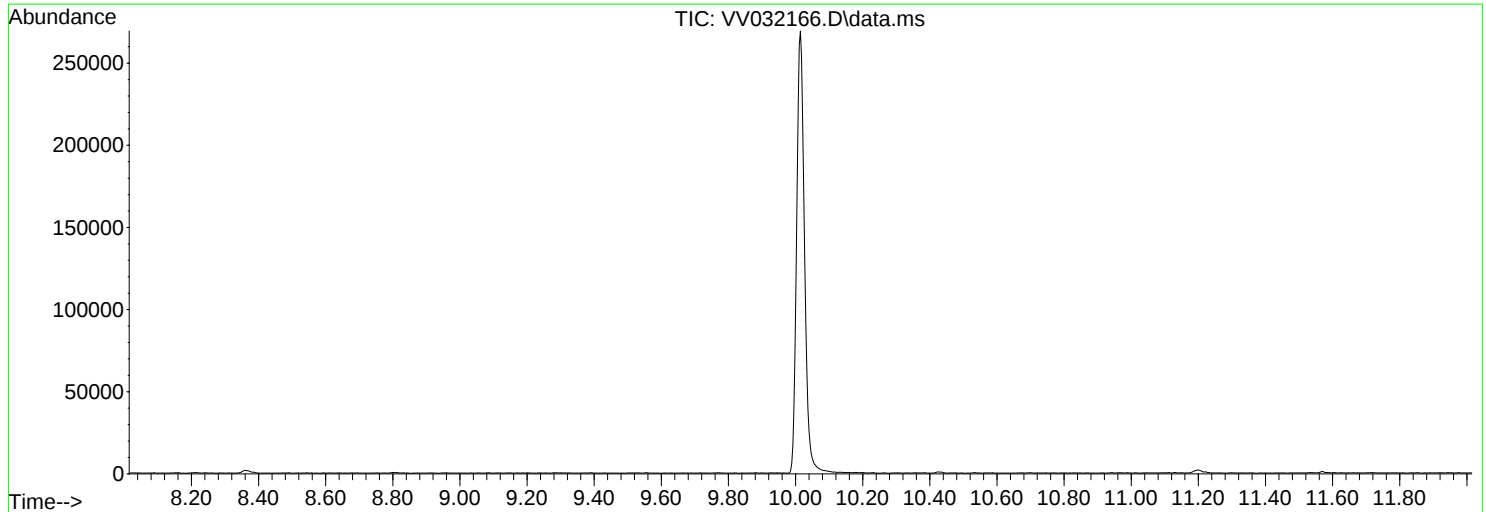

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	10107	PASS
75	95	30	80	50.8	27653	PASS
95	95	100	100	100.0	54424	PASS
96	95	5	9	6.6	3591	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.8	42339	PASS
175	174	5	9	7.3	3072	PASS
176	174	95	105	97.2	41160	PASS
177	176	5	10	6.5	2682	PASS

m/z	Abundance
39.80	185.0
43.90	302.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
36.00	499.0
37.00	2884.0
37.90	2351.0
39.00	907.0
39.90	217.0
43.90	698.0
45.00	472.0
46.90	700.0
47.90	454.0
49.00	2305.0
50.00	10121.0
51.00	3218.0
52.00	144.0
54.90	211.0
56.00	786.0
56.90	1503.0
59.90	570.0
61.00	2889.0
62.00	2580.0
63.00	1898.0
63.80	179.0
64.90	177.0
66.90	185.0
68.00	5184.0
69.00	5939.0
70.00	425.0
71.90	431.0
73.00	2641.0
74.00	9394.0
75.00	27912.0
76.00	2393.0
77.00	448.0
78.00	265.0
78.90	1714.0
79.80	512.0
80.90	1698.0
81.80	429.0
85.90	123.0
86.90	2385.0
87.90	2308.0
90.90	211.0
92.00	1634.0
93.00	2325.0
94.00	6400.0
95.00	54720.0
96.00	3552.0
96.90	124.0
103.90	267.0
104.90	117.0
105.80	309.0
115.90	181.0
116.80	366.0
117.80	214.0
118.90	370.0
127.90	207.0
128.90	108.0
129.80	191.0
130.90	106.0
134.80	100.0
140.90	517.0
142.90	596.0
147.70	113.0
154.80	178.0
171.90	268.0
173.90	41736.0
175.00	3058.0
175.90	40104.0
176.90	2764.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
36.10	471.0
37.00	2841.0
37.90	2390.0
39.00	821.0
39.80	242.0
43.90	698.0
45.00	525.0
46.20	104.0
46.90	733.0
48.00	499.0
49.00	2509.0
50.00	10432.0
51.00	3250.0
52.00	165.0
54.90	210.0
55.90	859.0
56.90	1537.0
59.90	571.0
61.00	2893.0
62.00	2634.0
62.90	1990.0
63.80	167.0
64.90	161.0
66.90	186.0
68.00	5305.0
69.00	5870.0
70.00	453.0
71.90	438.0
73.00	2721.0
74.00	9322.0
75.00	28360.0
76.00	2343.0
77.00	417.0
78.00	268.0
78.90	1771.0
79.80	545.0
80.90	1735.0
81.80	467.0
85.80	114.0
86.90	2492.0
87.90	2336.0
90.90	216.0
92.00	1735.0
93.00	2487.0
94.00	6449.0
95.00	56064.0
96.00	3727.0
97.00	124.0
103.80	288.0
104.80	108.0
105.90	331.0
115.90	182.0
116.80	389.0
117.80	219.0
118.90	366.0
127.80	219.0
128.80	108.0
129.90	220.0
130.90	133.0
134.80	103.0
136.90	112.0
140.90	515.0
142.90	658.0
147.80	131.0
154.80	190.0
171.90	288.0
173.90	43824.0
175.00	3106.0
175.90	42680.0
176.90	2762.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216

m/z	Abundance
36.00	423.0
37.00	2535.0
37.90	2256.0
39.00	725.0
39.80	241.0
42.70	105.0
43.90	638.0
45.00	567.0
46.90	673.0
48.00	470.0
49.00	2414.0
50.00	9768.0
51.00	3070.0
52.00	173.0
54.90	209.0
55.90	875.0
56.90	1449.0
59.90	499.0
61.00	2585.0
62.00	2464.0
62.90	1872.0
63.80	158.0
65.00	130.0
67.00	171.0
67.90	5165.0
69.00	5417.0
70.00	484.0
71.90	367.0
73.00	2518.0
74.00	8659.0
75.00	26688.0
76.00	2192.0
76.90	392.0
78.00	241.0
78.90	1678.0
79.80	560.0
80.90	1610.0
81.90	418.0
85.80	112.0
86.90	2336.0
87.90	2188.0
90.80	197.0
92.00	1574.0
93.00	2349.0
94.00	6046.0
95.00	52488.0
96.00	3495.0
96.90	122.0
103.80	296.0
104.80	106.0
105.90	326.0
115.80	189.0
116.80	352.0
117.80	237.0
118.80	321.0
127.80	195.0
128.80	117.0
129.90	215.0
130.90	135.0
134.70	102.0
136.90	116.0
140.90	487.0
142.90	662.0
147.80	136.0
154.80	182.0
172.00	257.0
173.90	41456.0
175.00	3052.0
175.90	40696.0
176.90	2520.0

Instrument :
MSVOA_V
ClientSampleId :
BFB216