

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037519.D
 Acq On : 25 Sep 2024 13:25
 Operator : SY/MD
 Sample : P4131-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 26 04:12:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 26 04:08:51 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	635406	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	614238	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	294630	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	210701	36.250	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	72.500%	
7) Chloroethane-d5	1.532	69	184643	41.103	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	82.200%	
11) 1,1-Dichloroethene-d2	2.060	65	97293	39.825	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	79.660%	
21) 2-Butanone-d5	3.793	46	201411	89.482	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	89.480%	
24) Chloroform-d	4.243	84	439743	48.339	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.680%	
26) 1,2-Dichloroethane-d4	4.937	65	270366	47.194	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	94.380%	
32) Benzene-d6	4.953	84	876716	47.256	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	94.520%	
36) 1,2-Dichloropropane-d6	5.982	67	281010	48.360	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	96.720%	
41) Toluene-d8	7.236	98	759045	45.333	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	90.660%	
43) trans-1,3-Dichloroprop...	7.551	79	121685	45.264	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	90.520%	
47) 2-Hexanone-d5	8.024	63	125321	79.023	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	79.020%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	318632	45.212	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	90.420%	
66) 1,2-Dichlorobenzene-d4	11.555	152	298556	50.595	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	101.200%	
Target Compounds						
13) Acetone	2.114	43	25119	10.406	ug/L	96
39) cis-1,3-Dichloropropene	6.908	75	7187	0.958	ug/L #	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037519.D
Acq On : 25 Sep 2024 13:25
Operator : SY/MD
Sample : P4131-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 26 04:12:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 04:08:51 2024
Response via : Initial Calibration

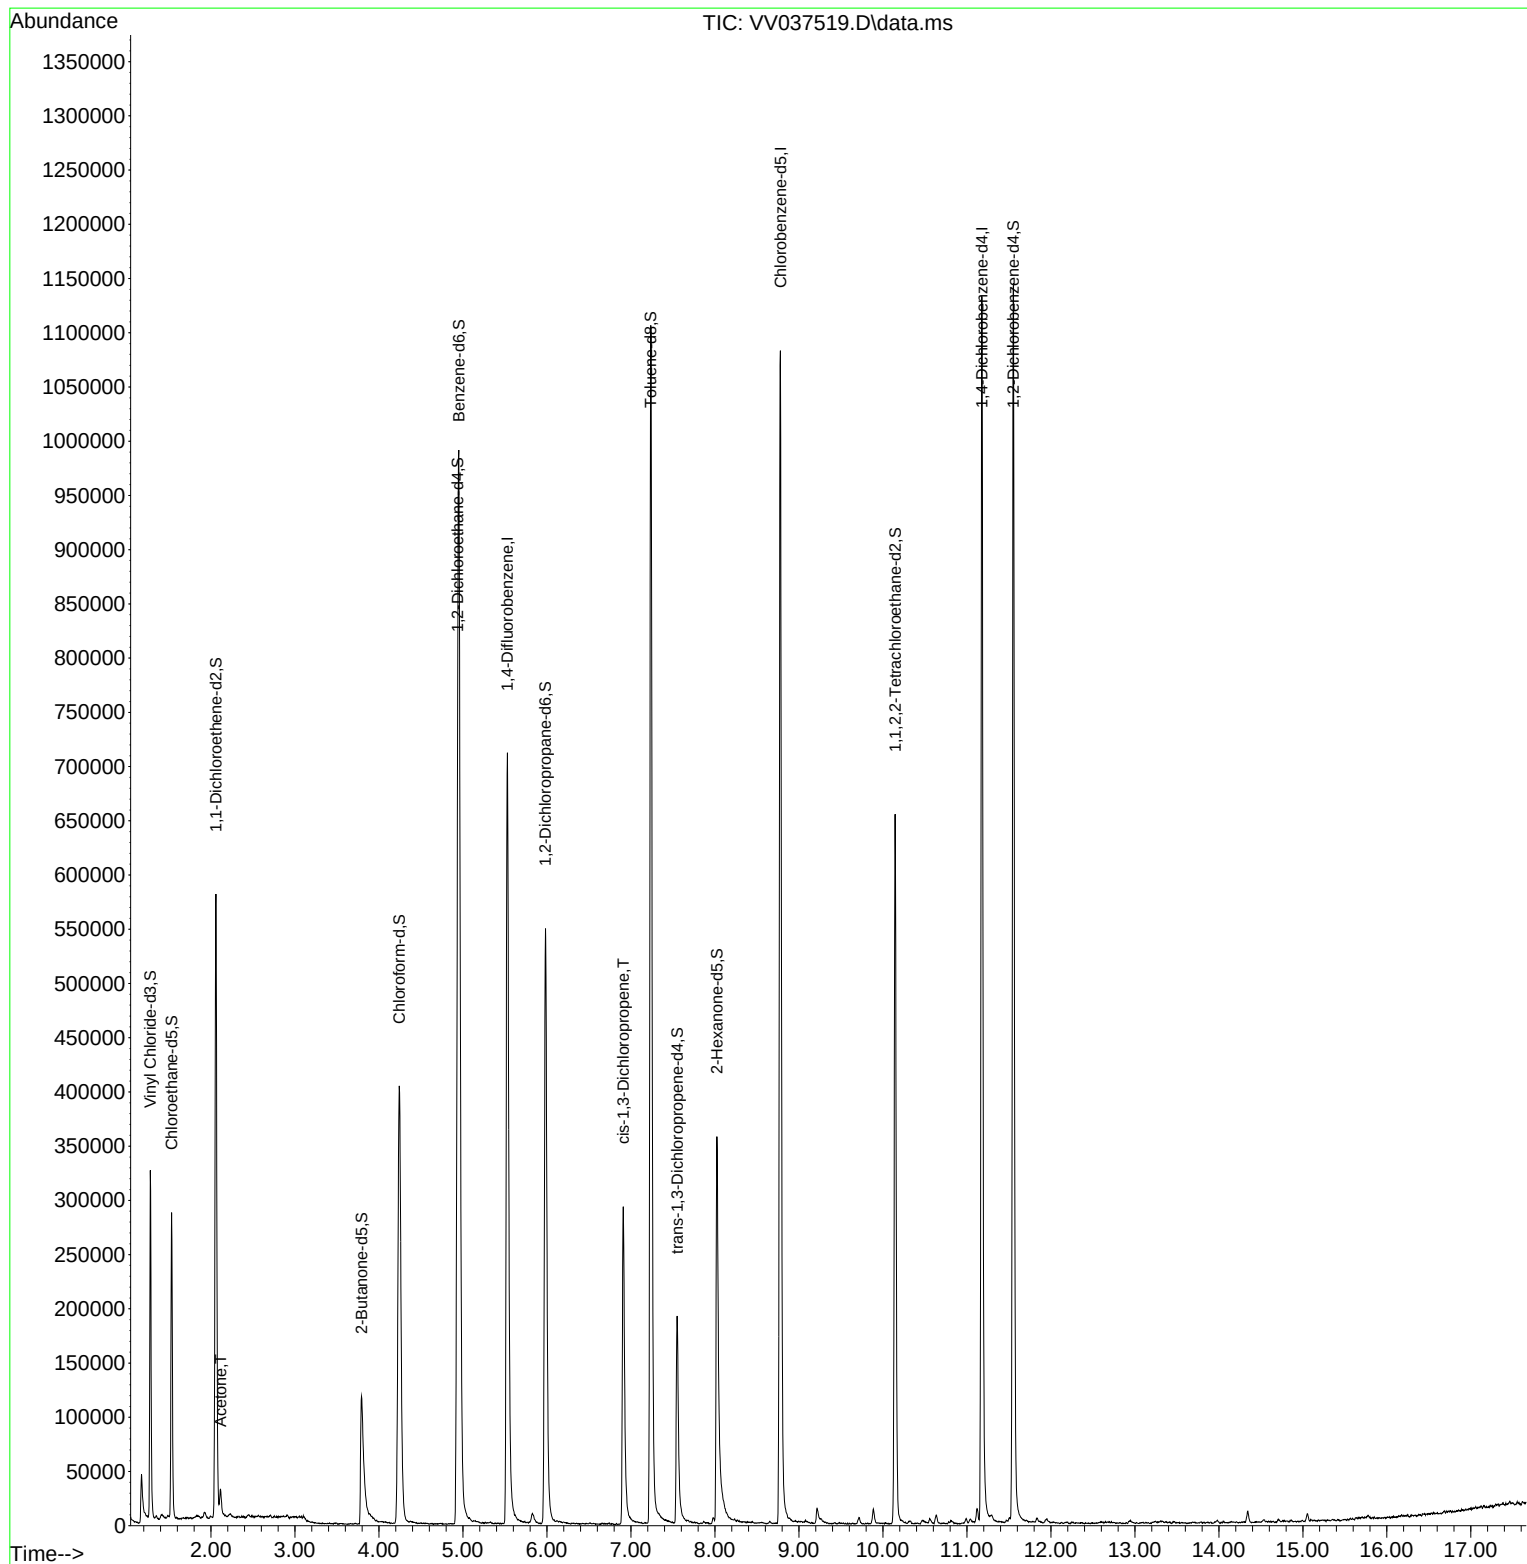

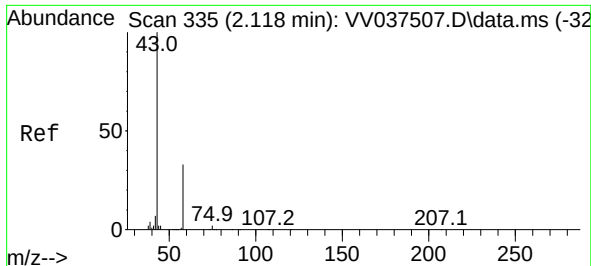

#13

Acetone

Concen: 10.406 ug/L

RT: 2.114 min Scan# 34

Delta R.T. -0.003 min

Lab File: VV037519.D

Acq: 25 Sep 2024 13:25

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 43 Resp: 25119

Ion Ratio Lower Upper

43 100

58 34.8 0.0 64.8

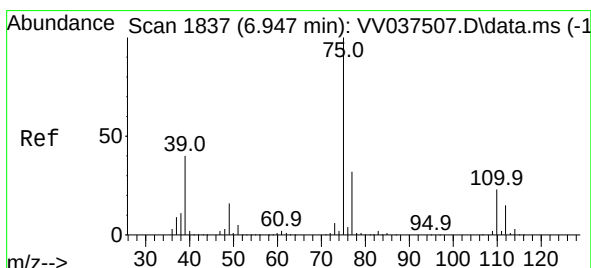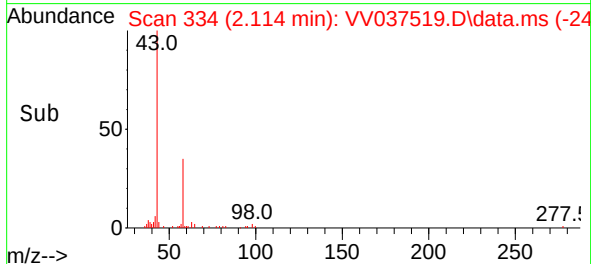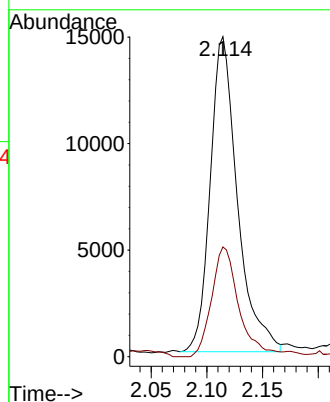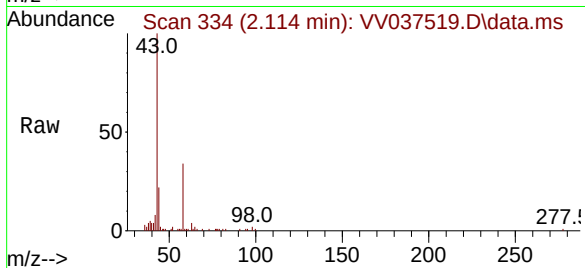

#39

cis-1,3-Dichloropropene

Concen: 0.958 ug/L

RT: 6.908 min Scan# 1825

Delta R.T. -0.038 min

Lab File: VV037519.D

Acq: 25 Sep 2024 13:25

Tgt Ion: 75 Resp: 7187

Ion Ratio Lower Upper

75 100

77 57.4 21.7 40.3#

