

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
 Data File : VV037527.D
 Acq On : 25 Sep 2024 16:17
 Operator : SY/MD
 Sample : P4183-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 26 04:14:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 26 04:08:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	622881	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	611808	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	293232	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	199418	34.999	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	70.000%
7) Chloroethane-d5	1.532	69	174868	39.710	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.420%
11) 1,1-Dichloroethene-d2	2.060	65	90504	37.791	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.580%
21) 2-Butanone-d5	3.793	46	190310	86.250	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.250%
24) Chloroform-d	4.243	84	410799	46.066	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.140%
26) 1,2-Dichloroethane-d4	4.937	65	248642	44.275	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.540%
32) Benzene-d6	4.953	84	800041	43.295	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.580%
36) 1,2-Dichloropropane-d6	5.982	67	262870	45.418	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.840%
41) Toluene-d8	7.239	98	692407	41.518	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	83.040%
43) trans-1,3-Dichloroprop...	7.551	79	109409	40.859	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.720%
47) 2-Hexanone-d5	8.024	63	120149	76.062	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	76.060%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	309600	44.105	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.220%
66) 1,2-Dichlorobenzene-d4	11.554	152	279373	47.570	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.140%
Target Compounds						
					Qvalue	
13) Acetone	2.114	43	26139	11.046	ug/L	98
39) cis-1,3-Dichloropropene	6.905	75	7323	0.980	ug/L #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092524\
Data File : VV037527.D
Acq On : 25 Sep 2024 16:17
Operator : SY/MD
Sample : P4183-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Sep 26 04:14:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 04:08:51 2024
Response via : Initial Calibration

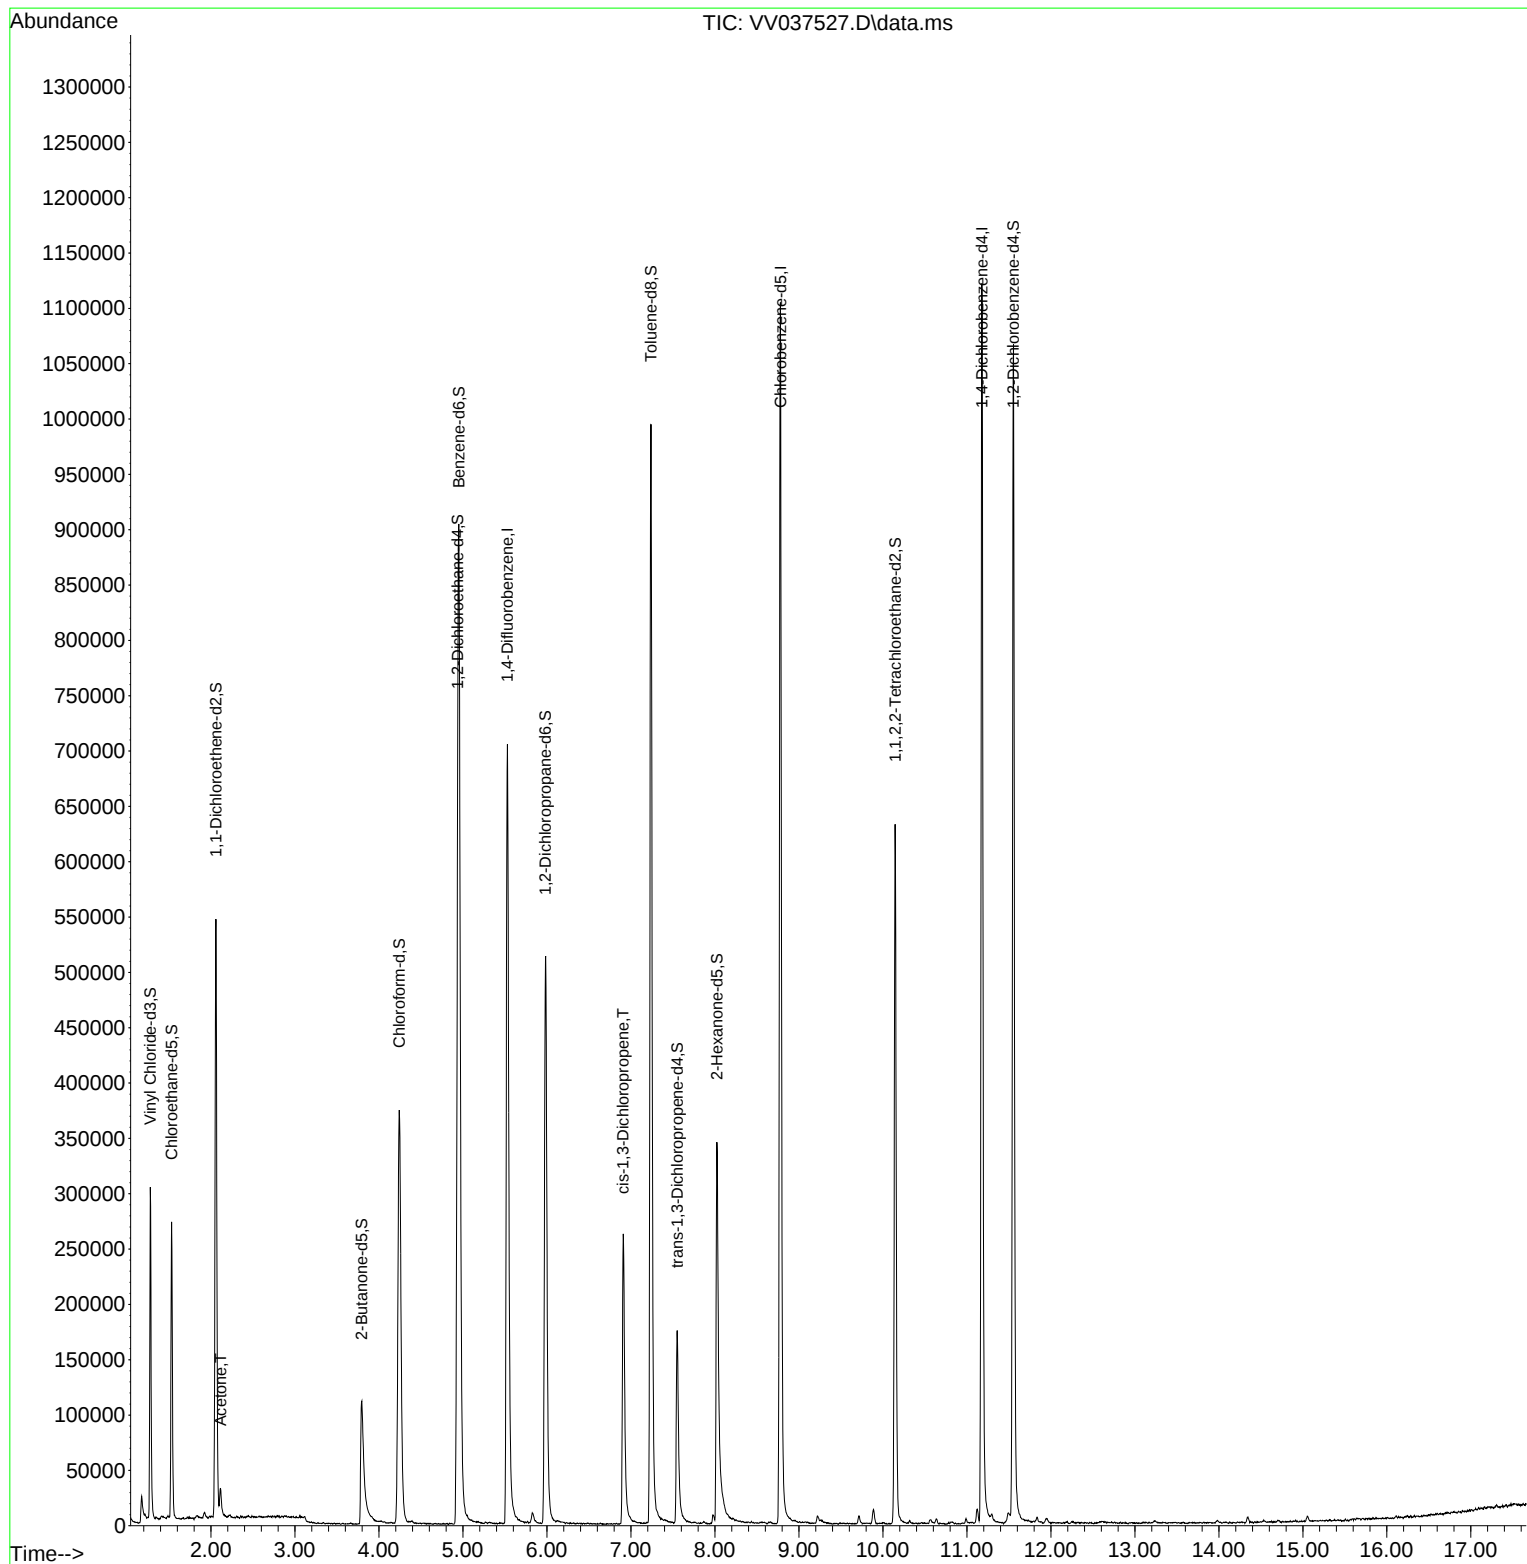



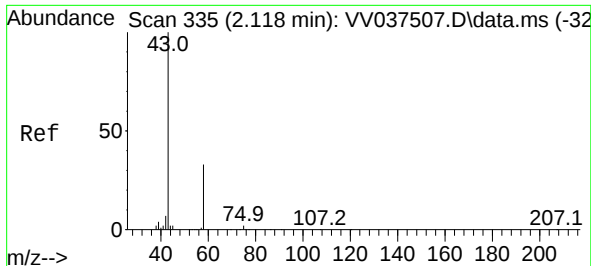


#13
Acetone
Concen: 11.046 ug/L
RT: 2.114 min Scan# 34
Delta R.T. -0.003 min
Lab File: VV037527.D
Acq: 25 Sep 2024 16:17

Instrument :
MSVOA_V
ClientSampleId :

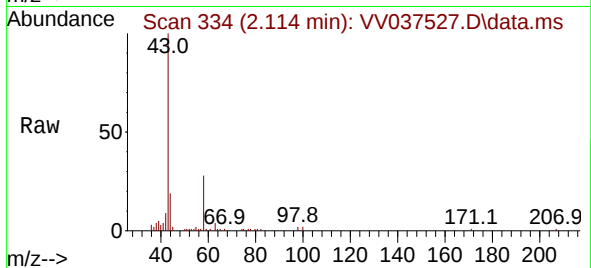

Tgt Ion: 43 Resp: 26139
Ion Ratio Lower Upper
43 100
58 33.3 0.0 64.8

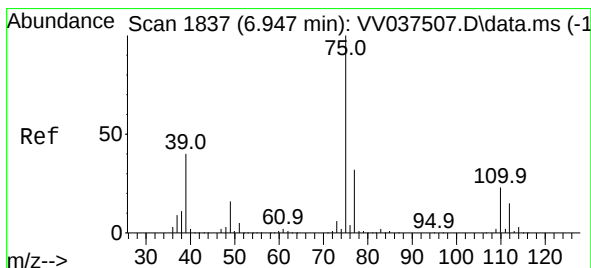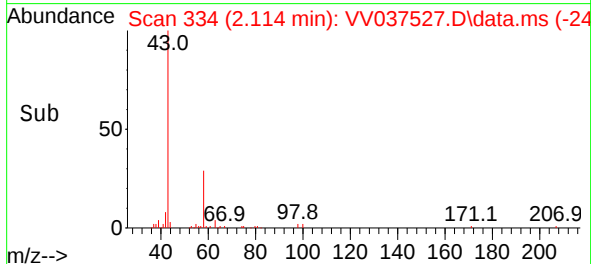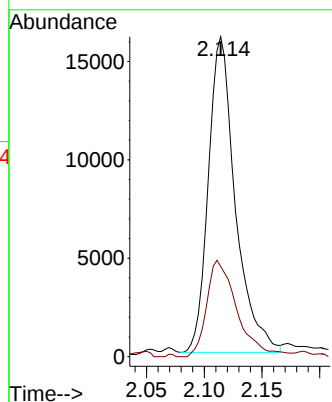

#39
cis-1,3-Dichloropropene
Concen: 0.980 ug/L
RT: 6.905 min Scan# 1824
Delta R.T. -0.042 min
Lab File: VV037527.D
Acq: 25 Sep 2024 16:17

Tgt Ion: 75 Resp: 7323
Ion Ratio Lower Upper
75 100
77 48.1 21.7 40.3#

